


2025-07-29 09:33:19
ID:
Nome:

Emmanuelle Correia de Brito Lima

Impressão de 12Canais
Freq. Cardíaca: 55 bpm

Hospital: SESI
Confirmado por:

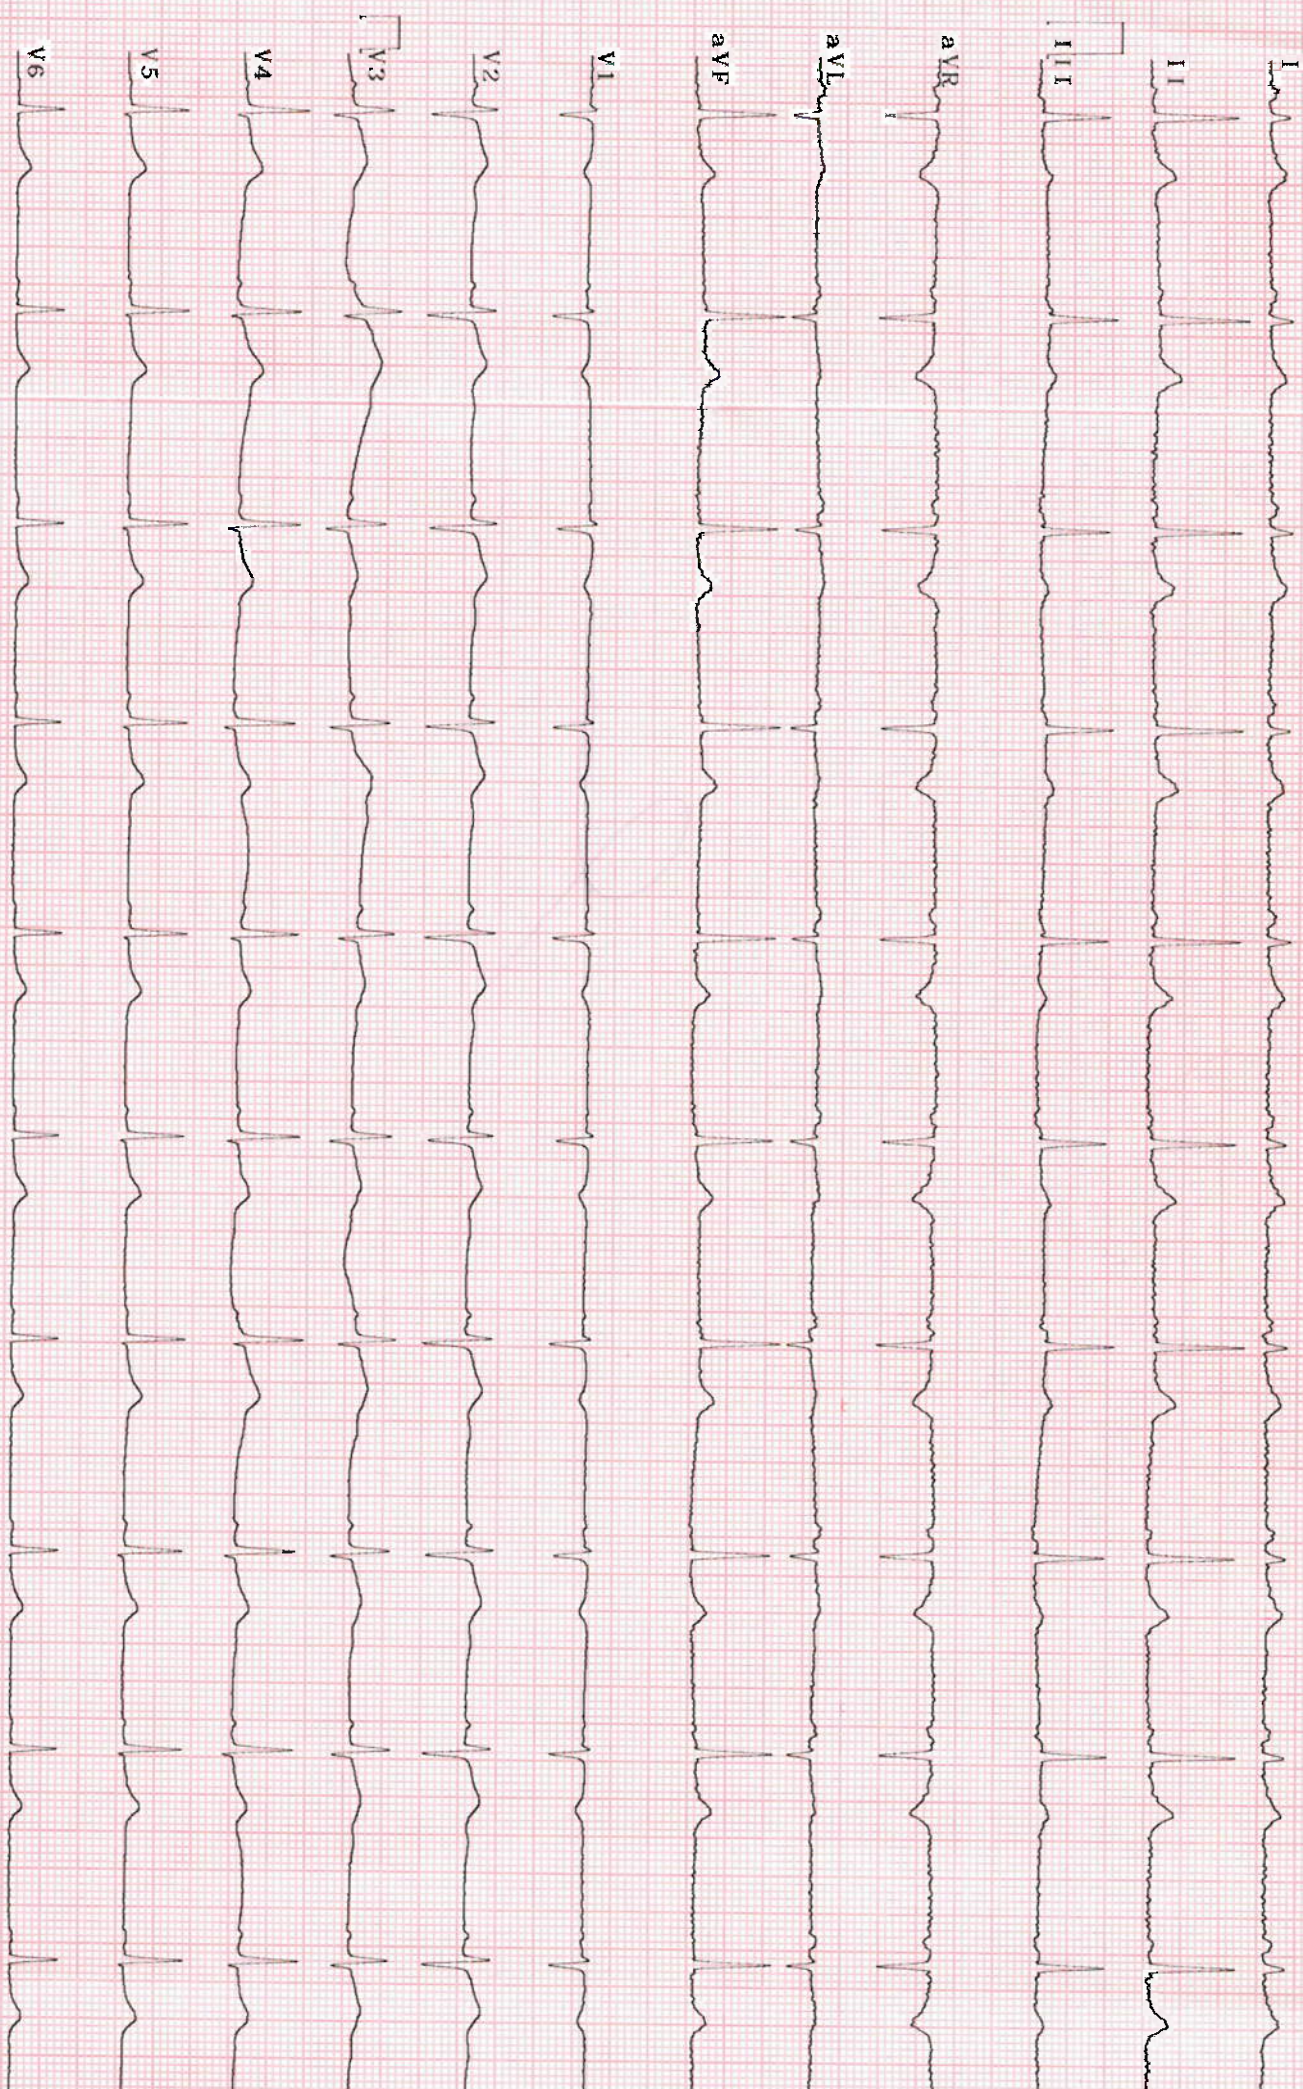

0.1Hz - 40Hz.

I-aVF:10.0mm/mV, V1-V6:5.0mm/mV, 25.0mm/seg.

CardioTouch6.11.30 Bionet Co.,Ltd.