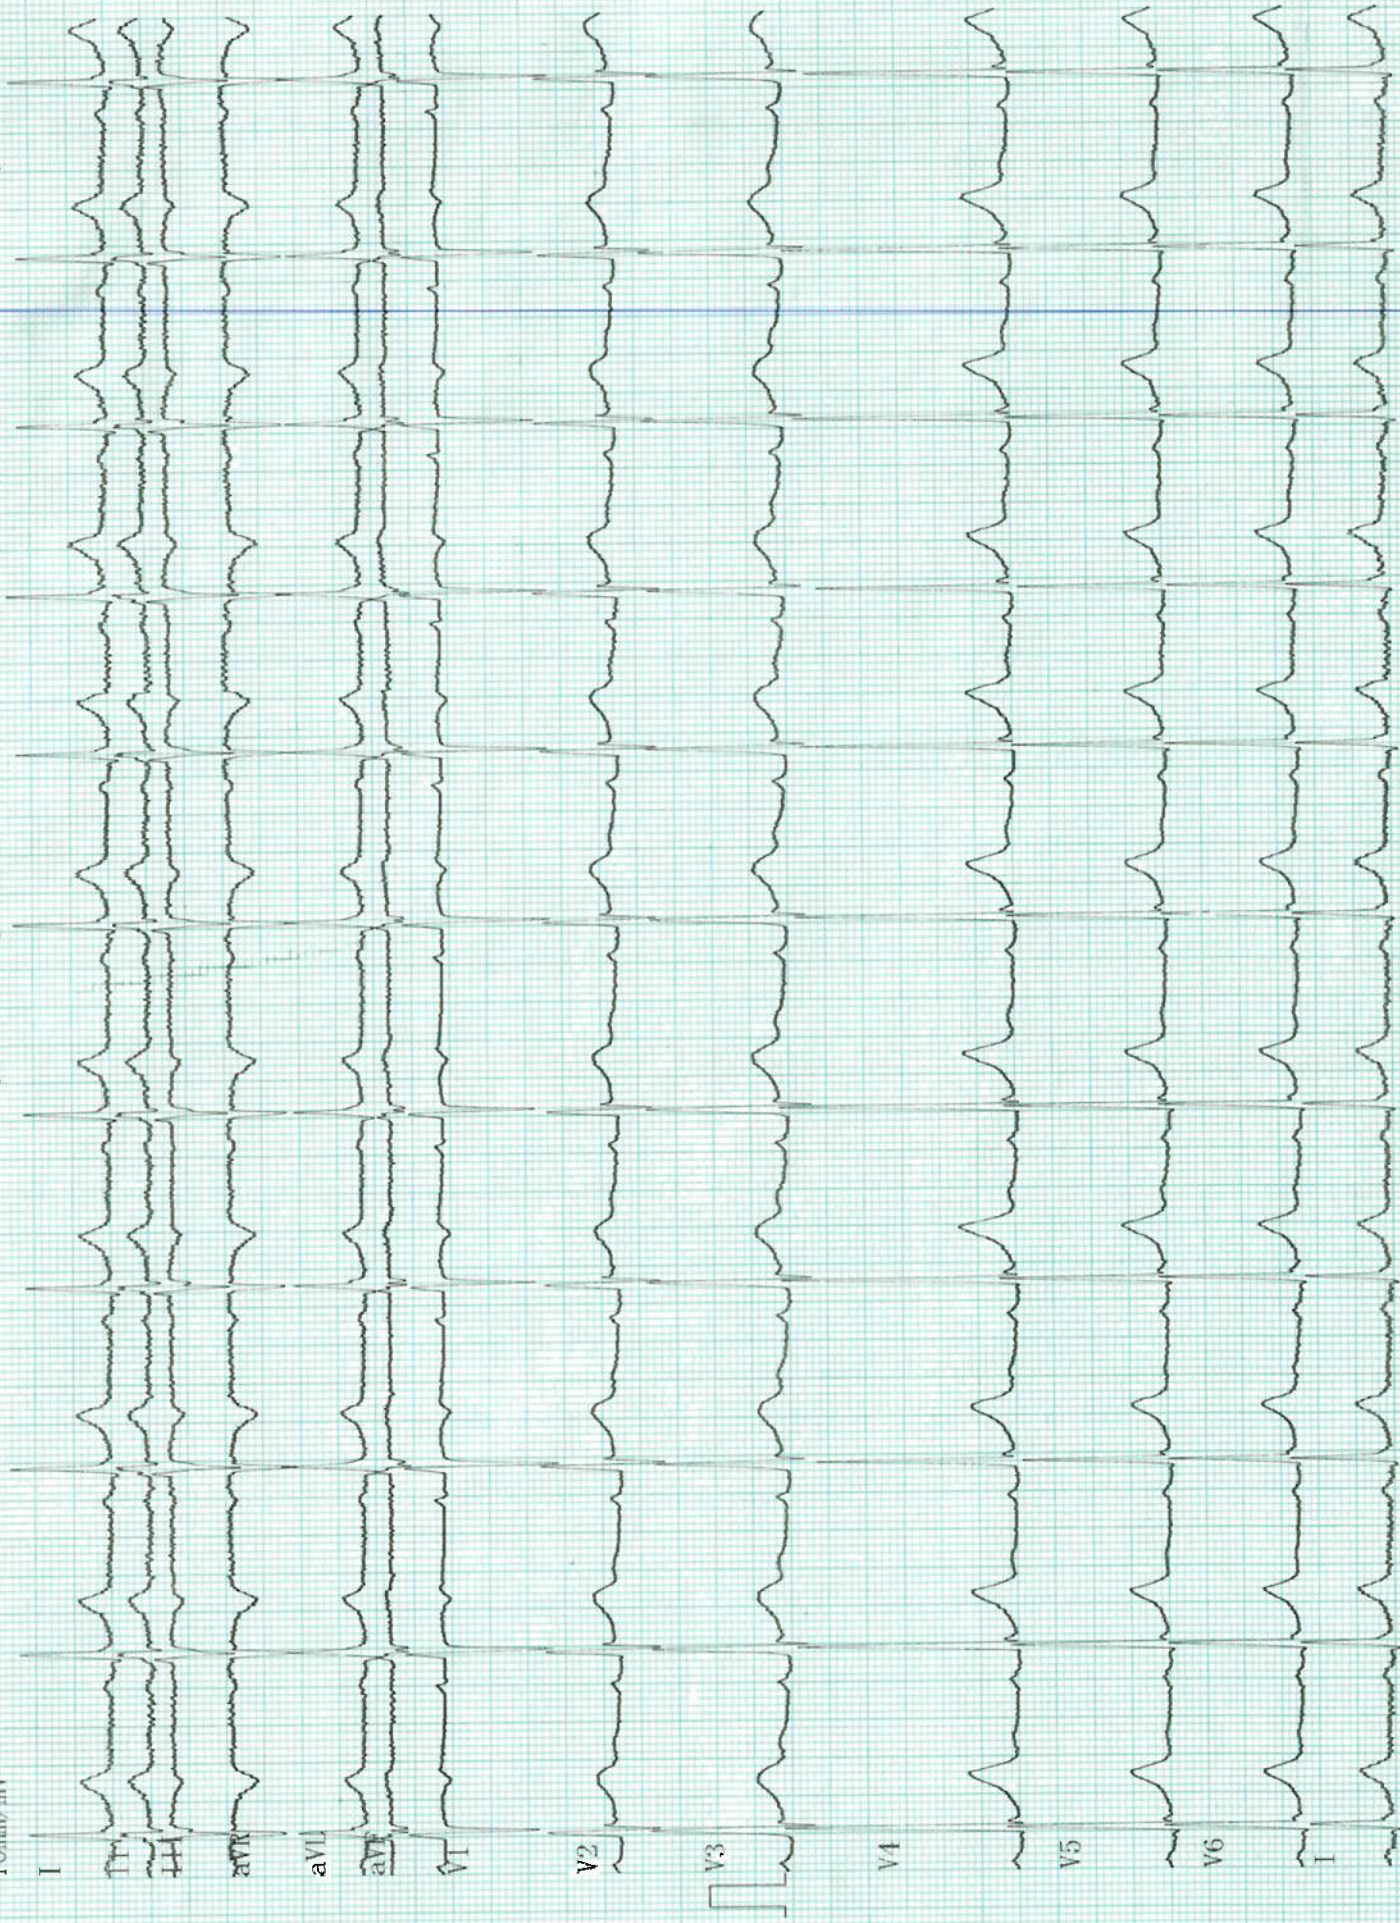


2025-08-08, 10:05
10mm/mV

Real-Time Mode

Leomando Ferreira do Nanto DN.25/01/1996

 $\text{Au}^{3+}/\text{AuHClO}_4$ 

Velocidade: 25mm/s	Filter: 150 d	35Hz	AC: 50 Hz	BIOCARE	ECG-1200	V4.06.000
--------------------	---------------	------	-----------	---------	----------	-----------