


2023 08 05, 10:36 Real Tempo Modo 10mm/mV

João Lopes de S. Filho

DN. 12101976

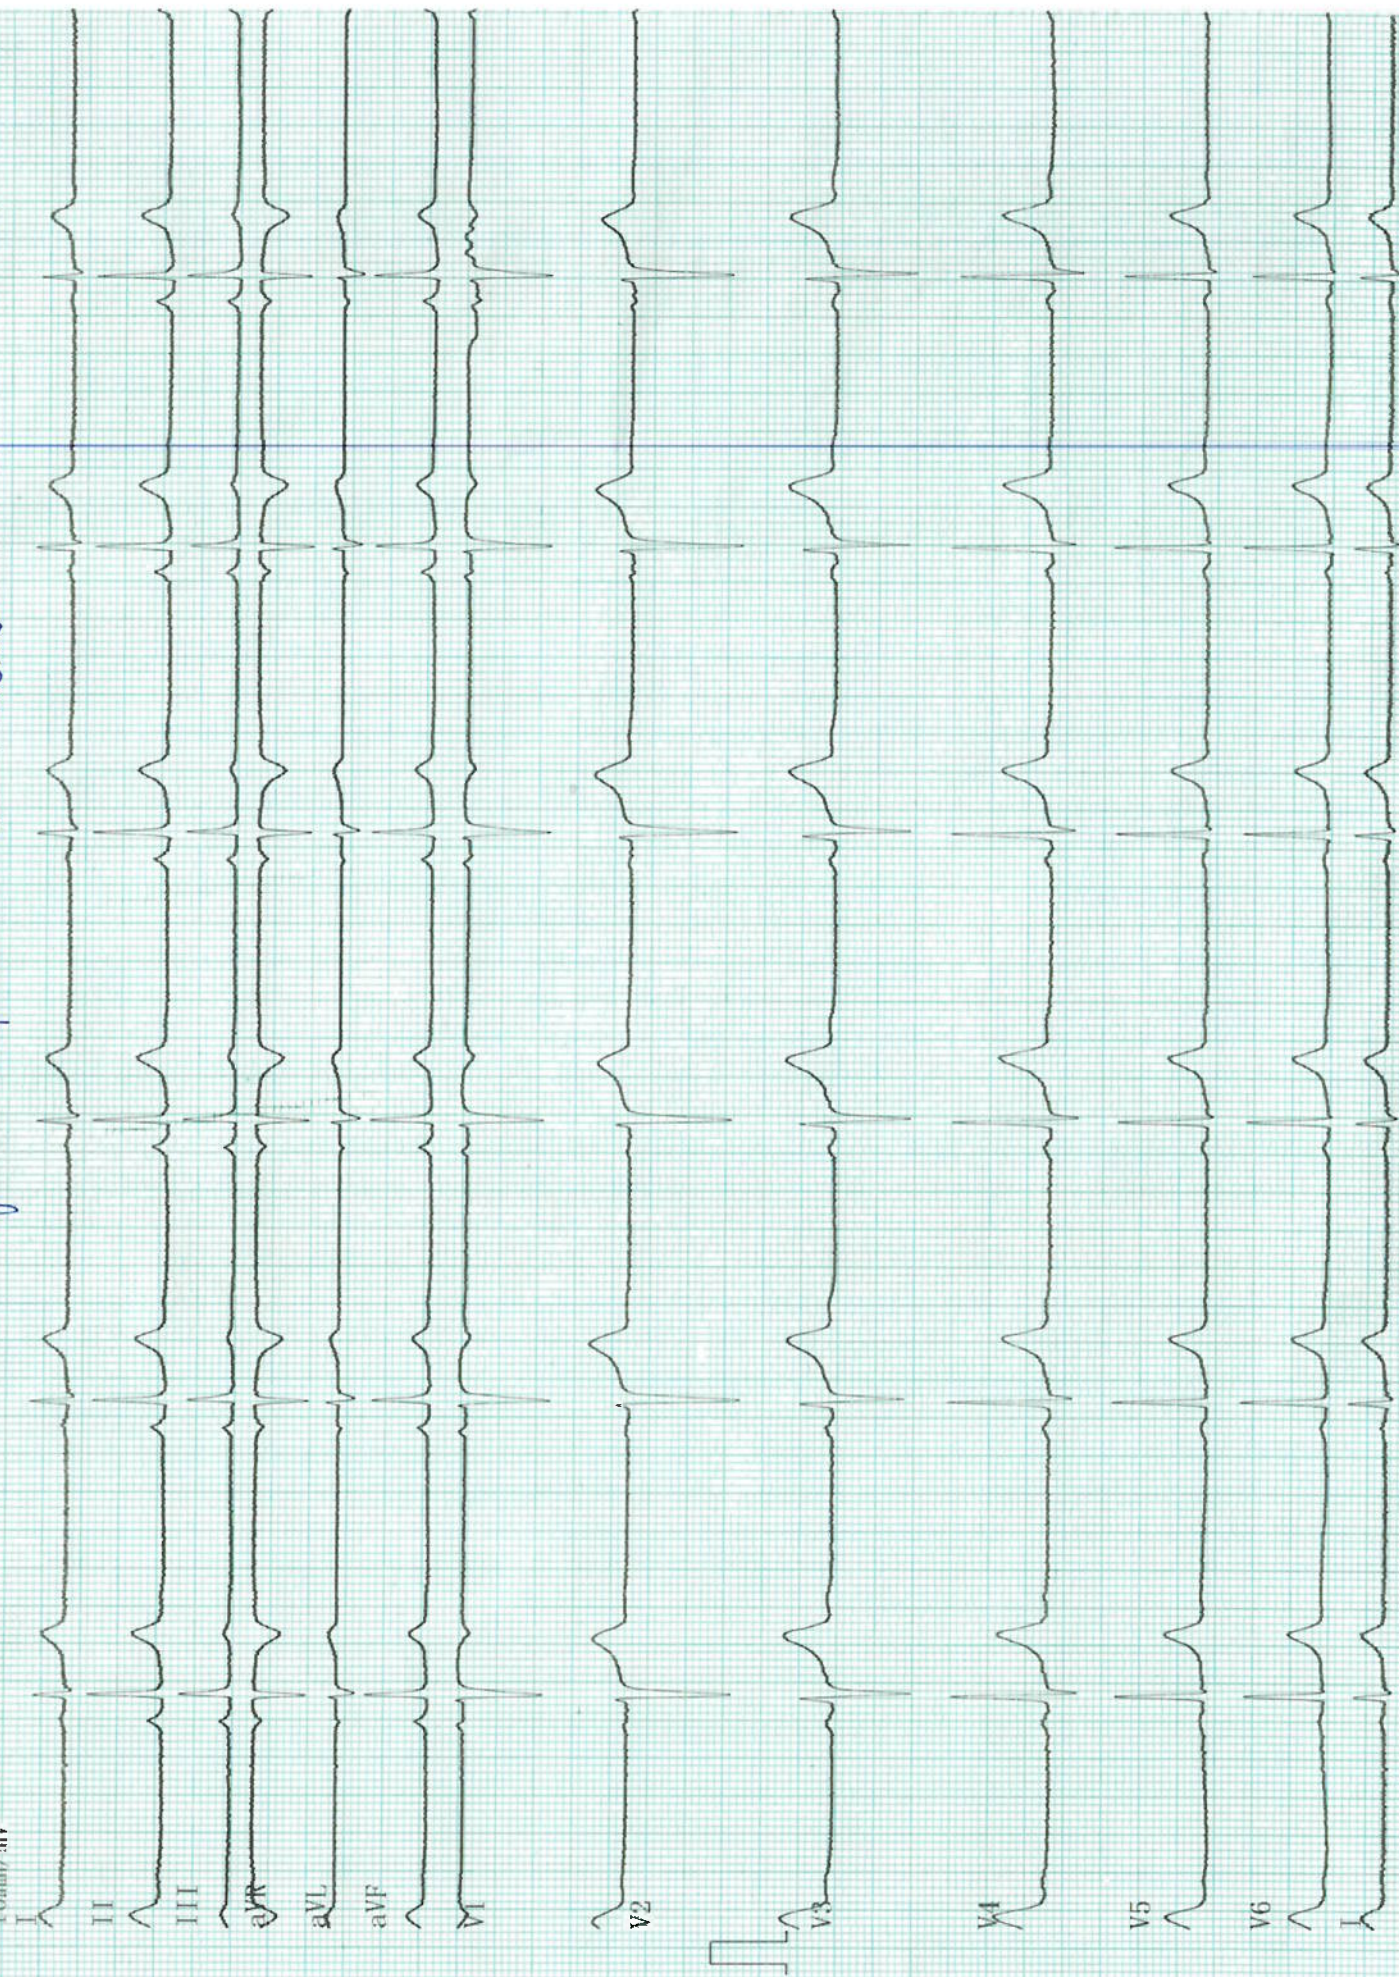

Velocidade: 25mm/s Filtro: H50 d 35Hz AC: 50 Hz BIO CARE ECG 1200 V4.06.000