


29/03/2024, 12:04 Real-Tempo Modo Lú3 Fernando Farias da Silva DN. 07/12/1991

10mm/mV

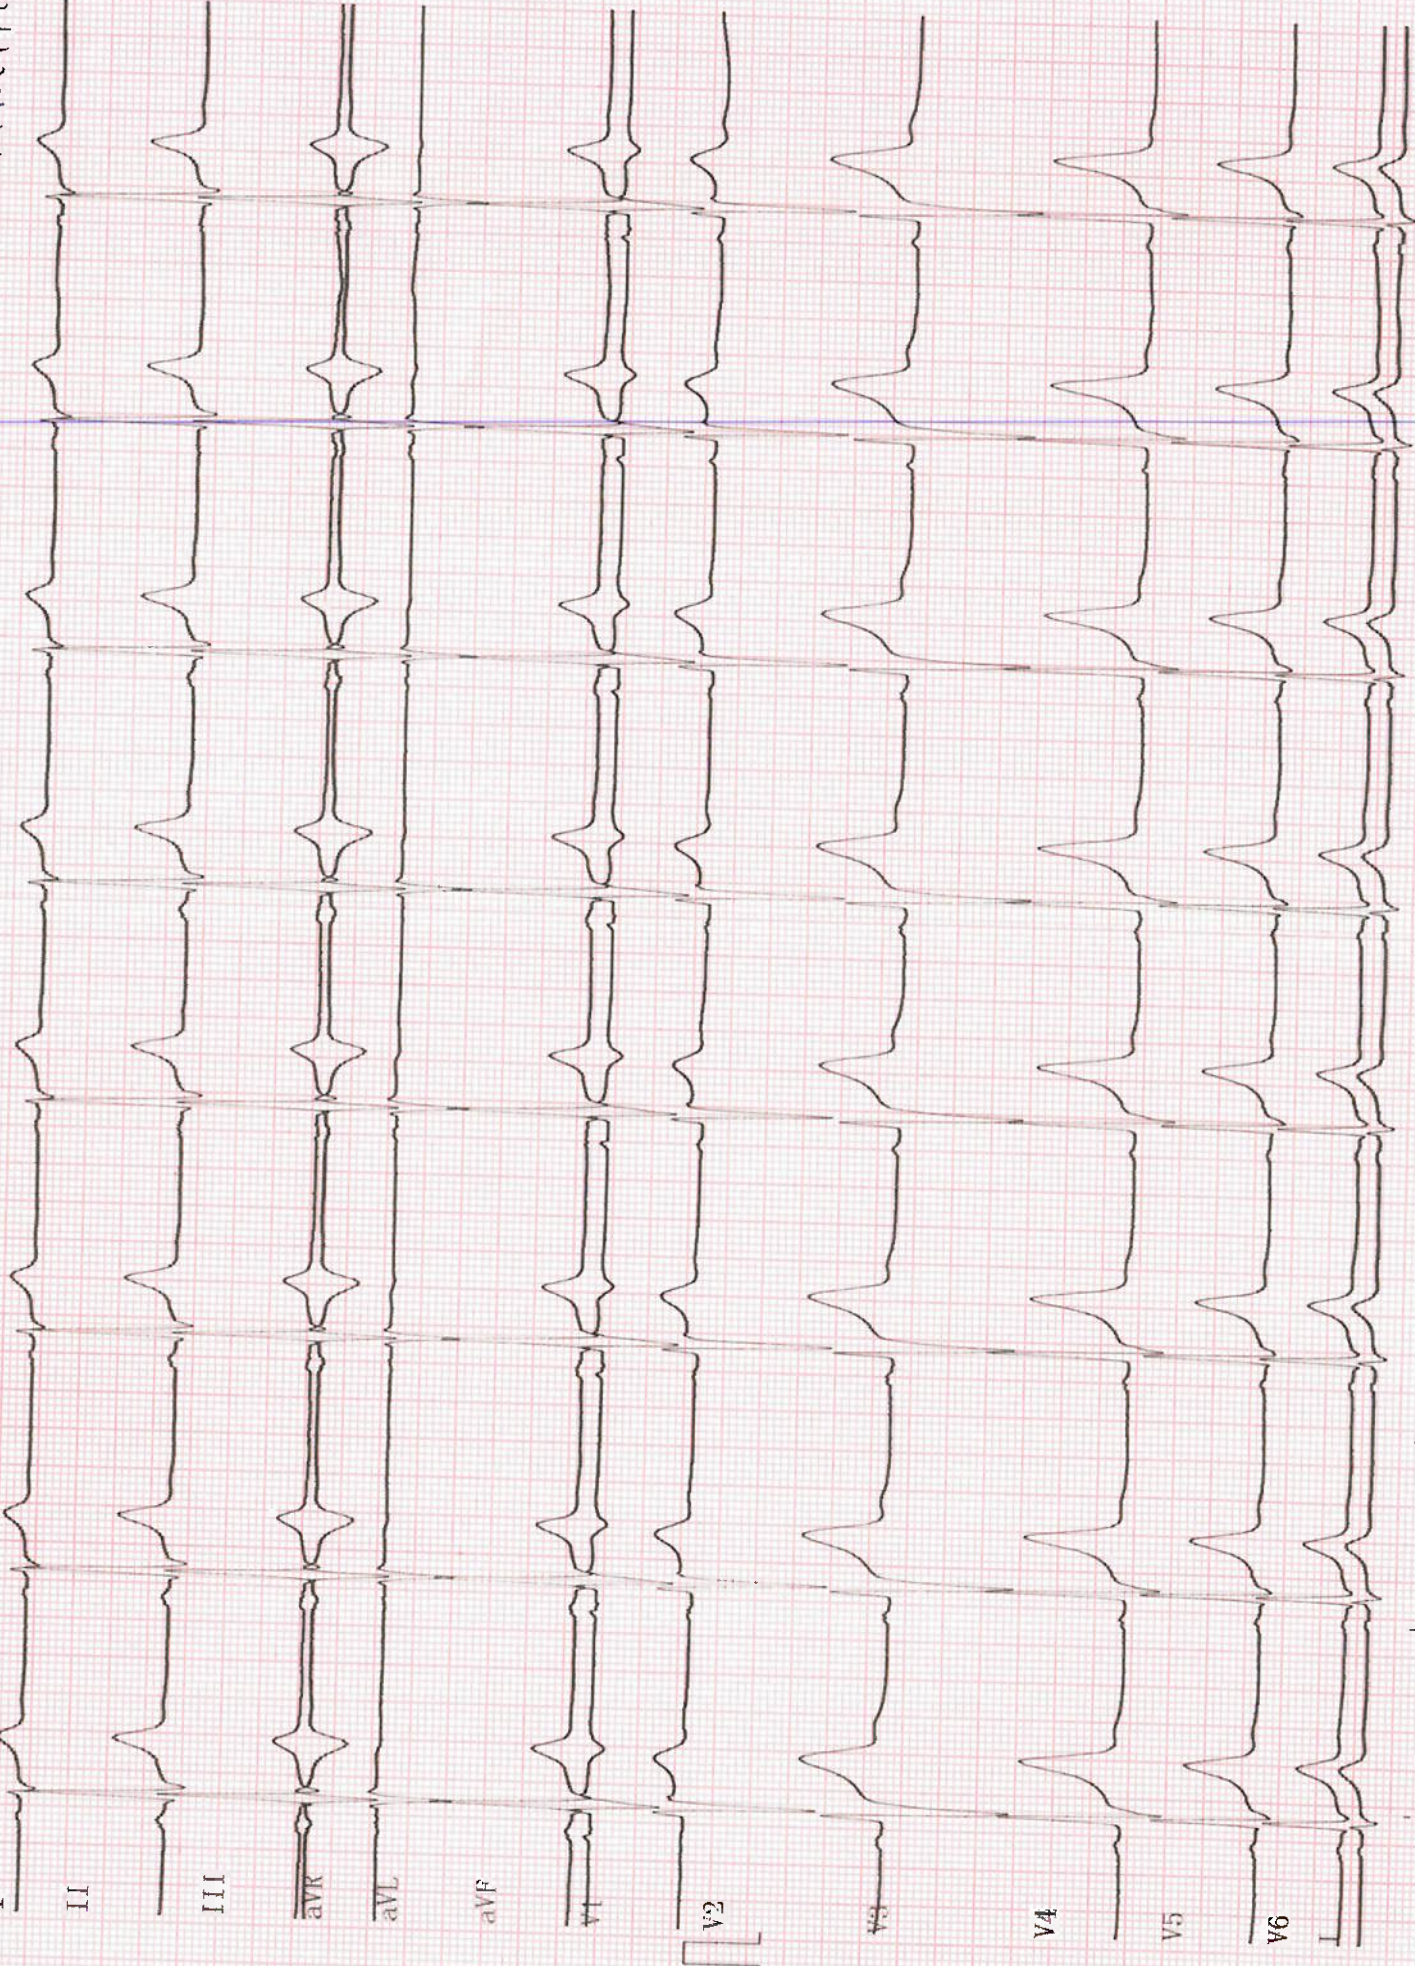

Velocidade: 25mm/s Filtro: H50 d 35Hz AC: 50 Hz BIO CARE ECG-1200 V4.06.000