

DN-0211211970


João da Silva

Manual

Real-Tempo Modo

2025 08 01, 09:01

10mm/mV

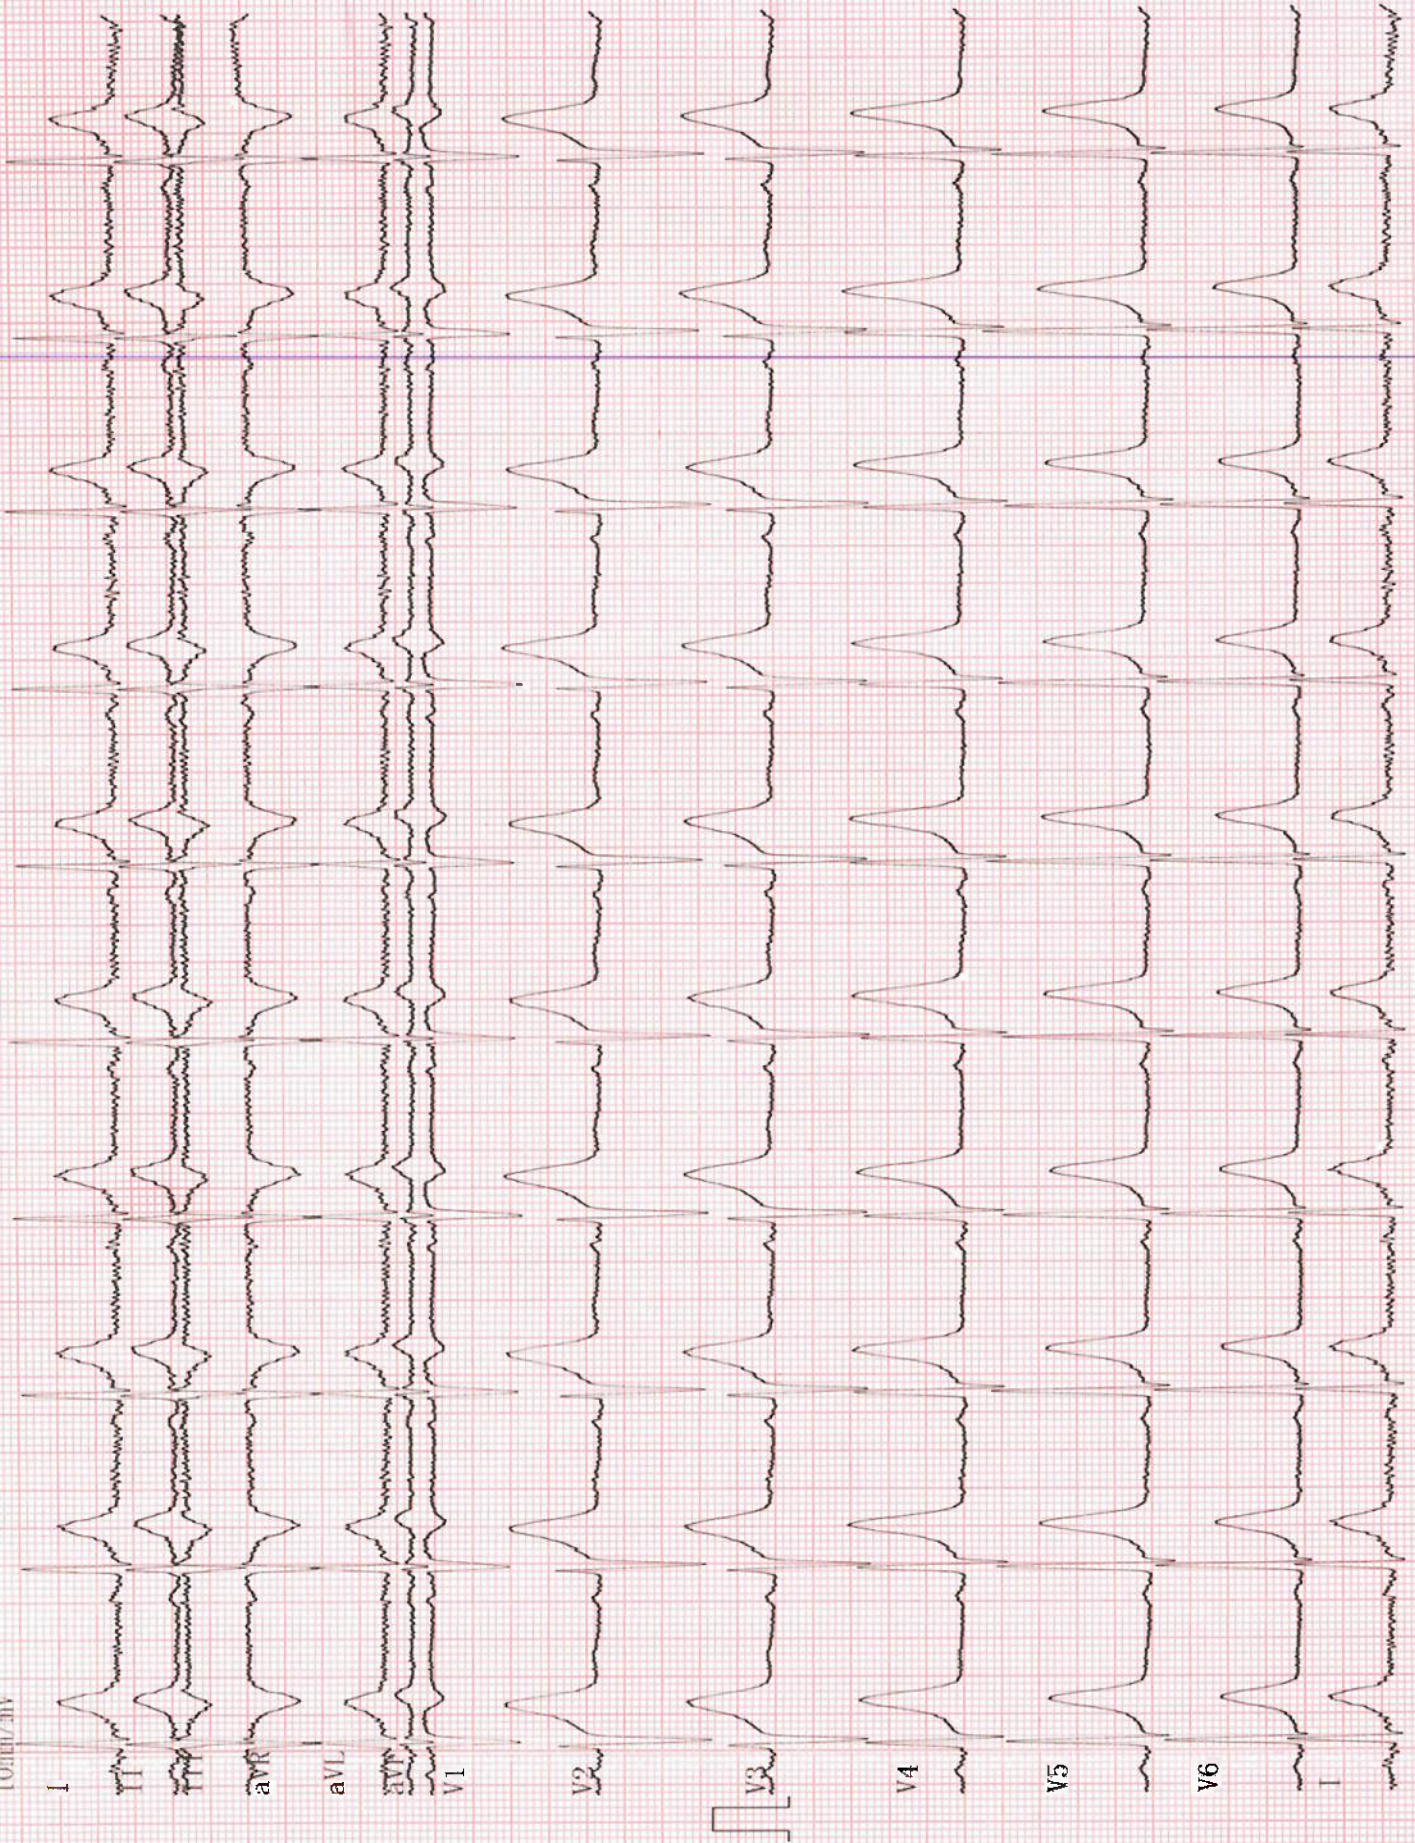

Velocidade: 25mm/s Filtro: H50 d 35Hz AC: 50 Hz BIOCARE ECG 1200 V4.06.000