


2025-08-08, 09:29
0mm/mV

Real-Tempo Modo

Ana Paula Campos de Lima DN- 12/03/1969

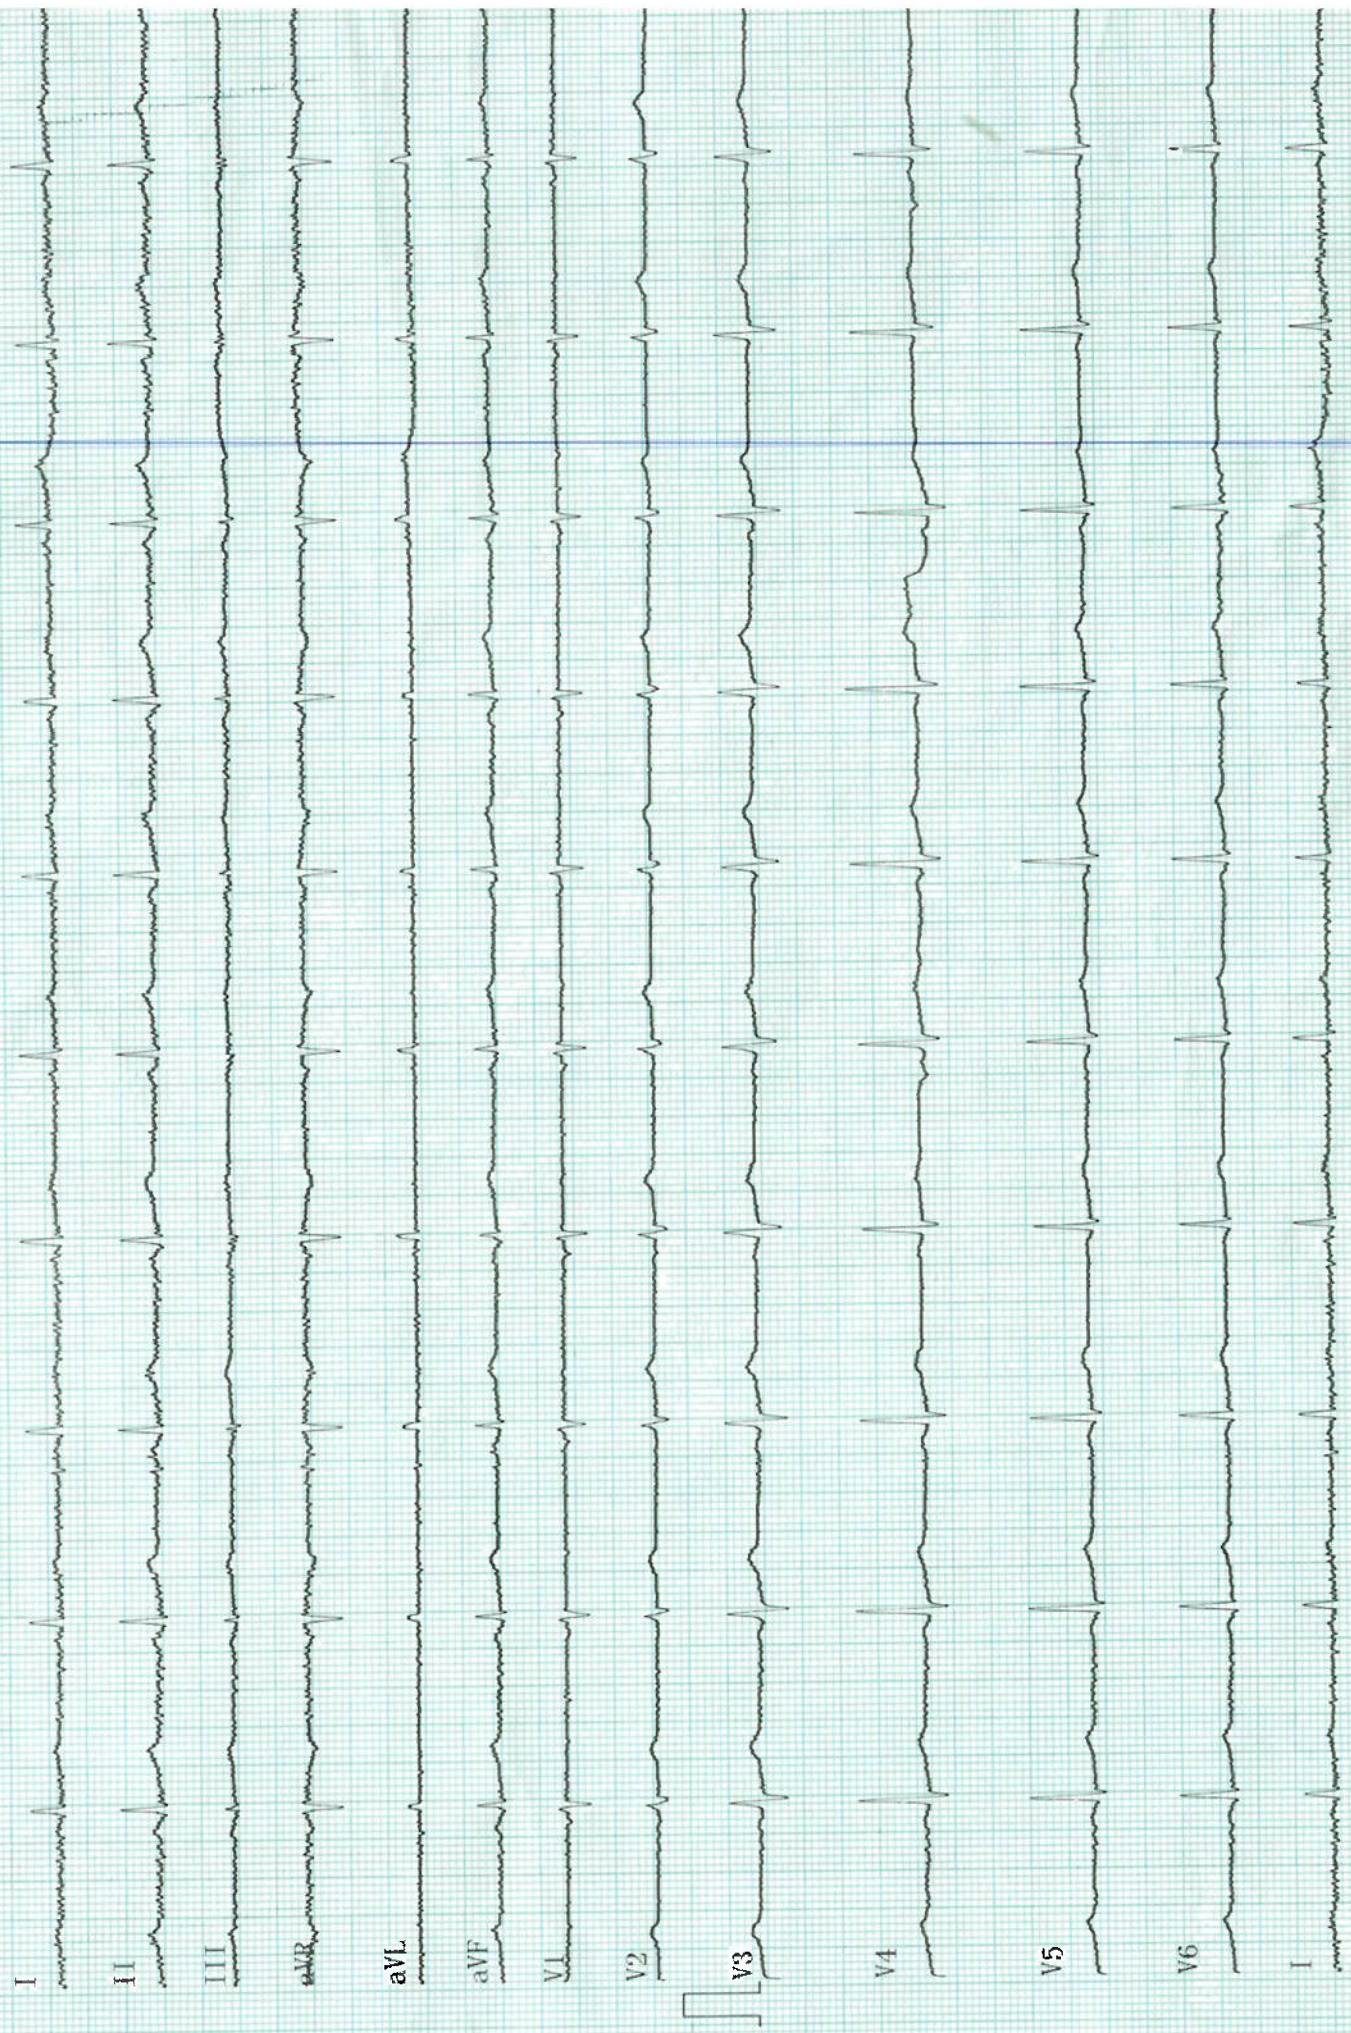

Velocidade: 25mm/s Filtro: H50 d 35Hz AC: 50 Hz BIOCARD ECG-1200 V4.06.000