


João Soutinho Alexandre DN. 05/05/1976

2025-08-05, 09:00
10mm/mV

Real Tempo Modo

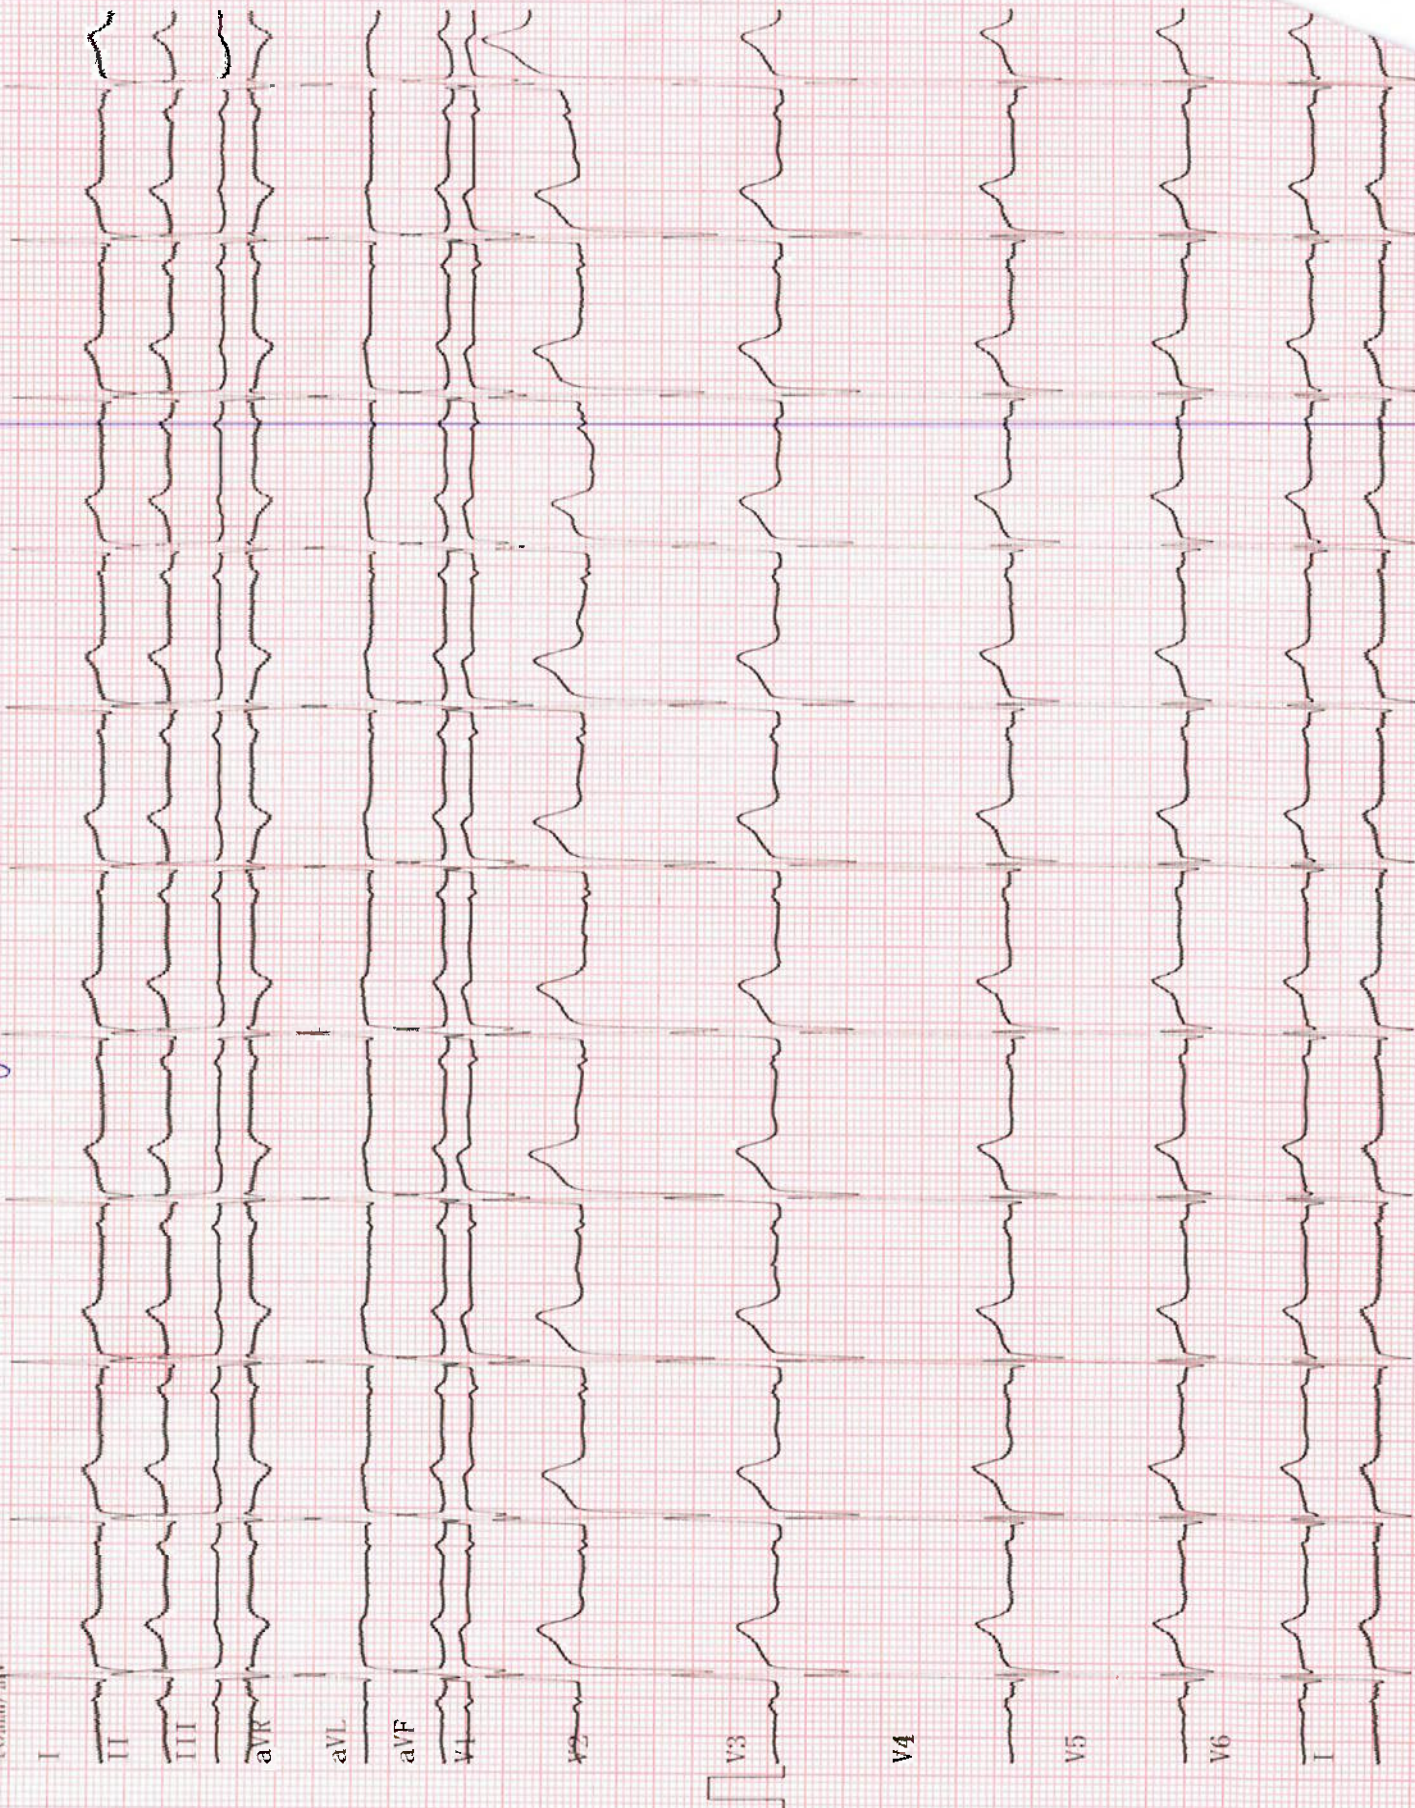

Velocidade: 25mm/s Filtro: 450 d 35Hz AC: 50 Hz BIOCARE ECG-1200 V4.06.000