


DN. 20108/1984

Edwardo Pedro Felix

Real-Tempo Modo

2025-08-01, 09:27

2025-08-10 AM 10:01

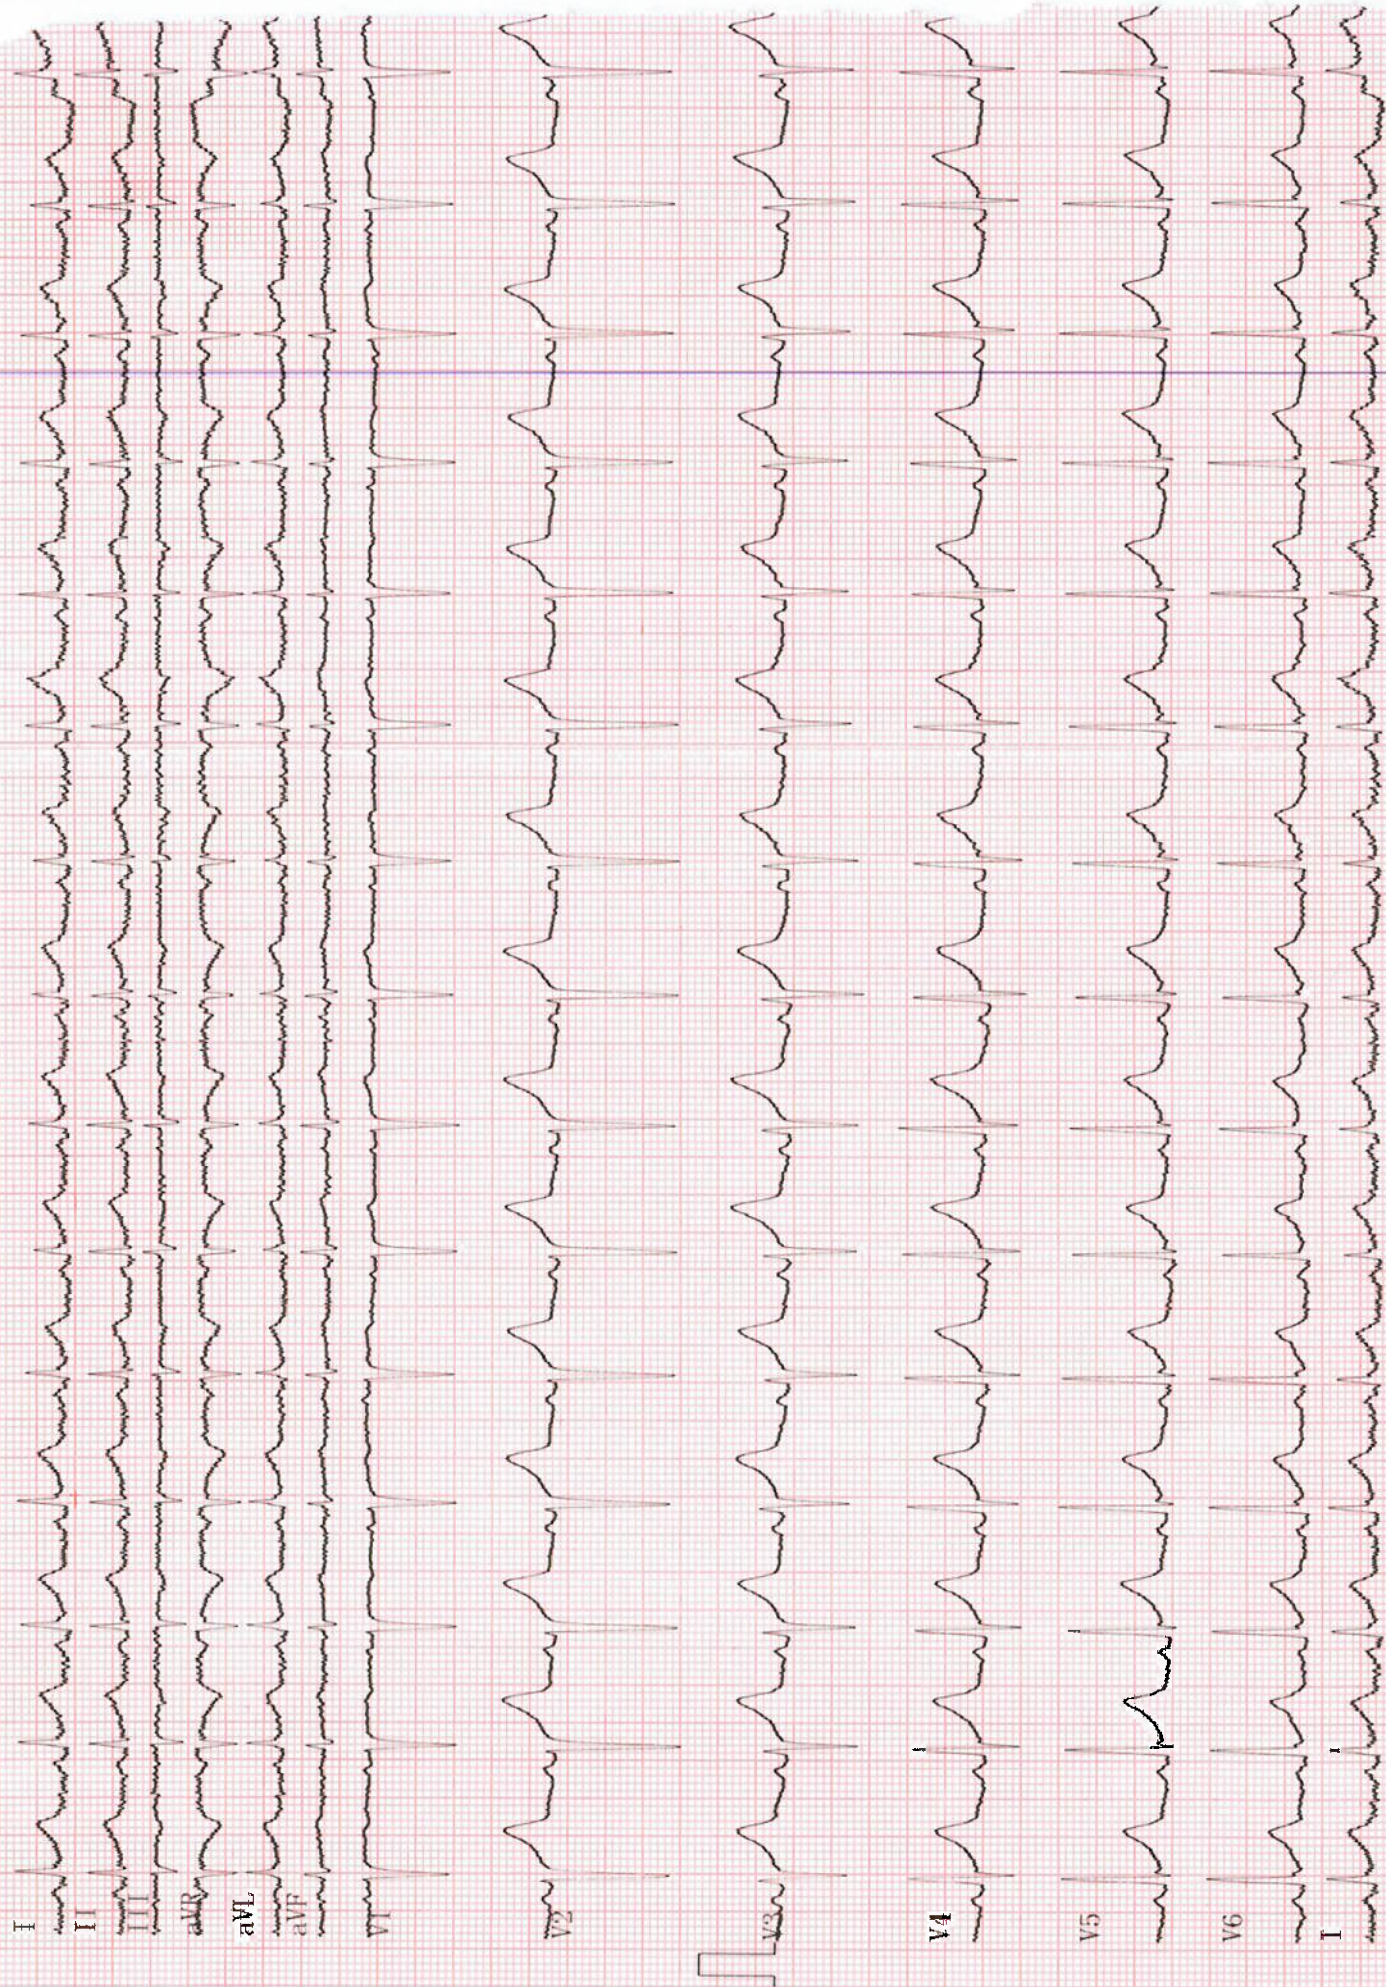

Velocidade: 25mm/s Filtro: 1150 d 35Hz AC: 50 Hz BIOCARE ECG-1200 V4.06.0000