


2025-07-22, 08:20

Real Tempo Modo

duis gel do sonder 56 ands

10mm/mV

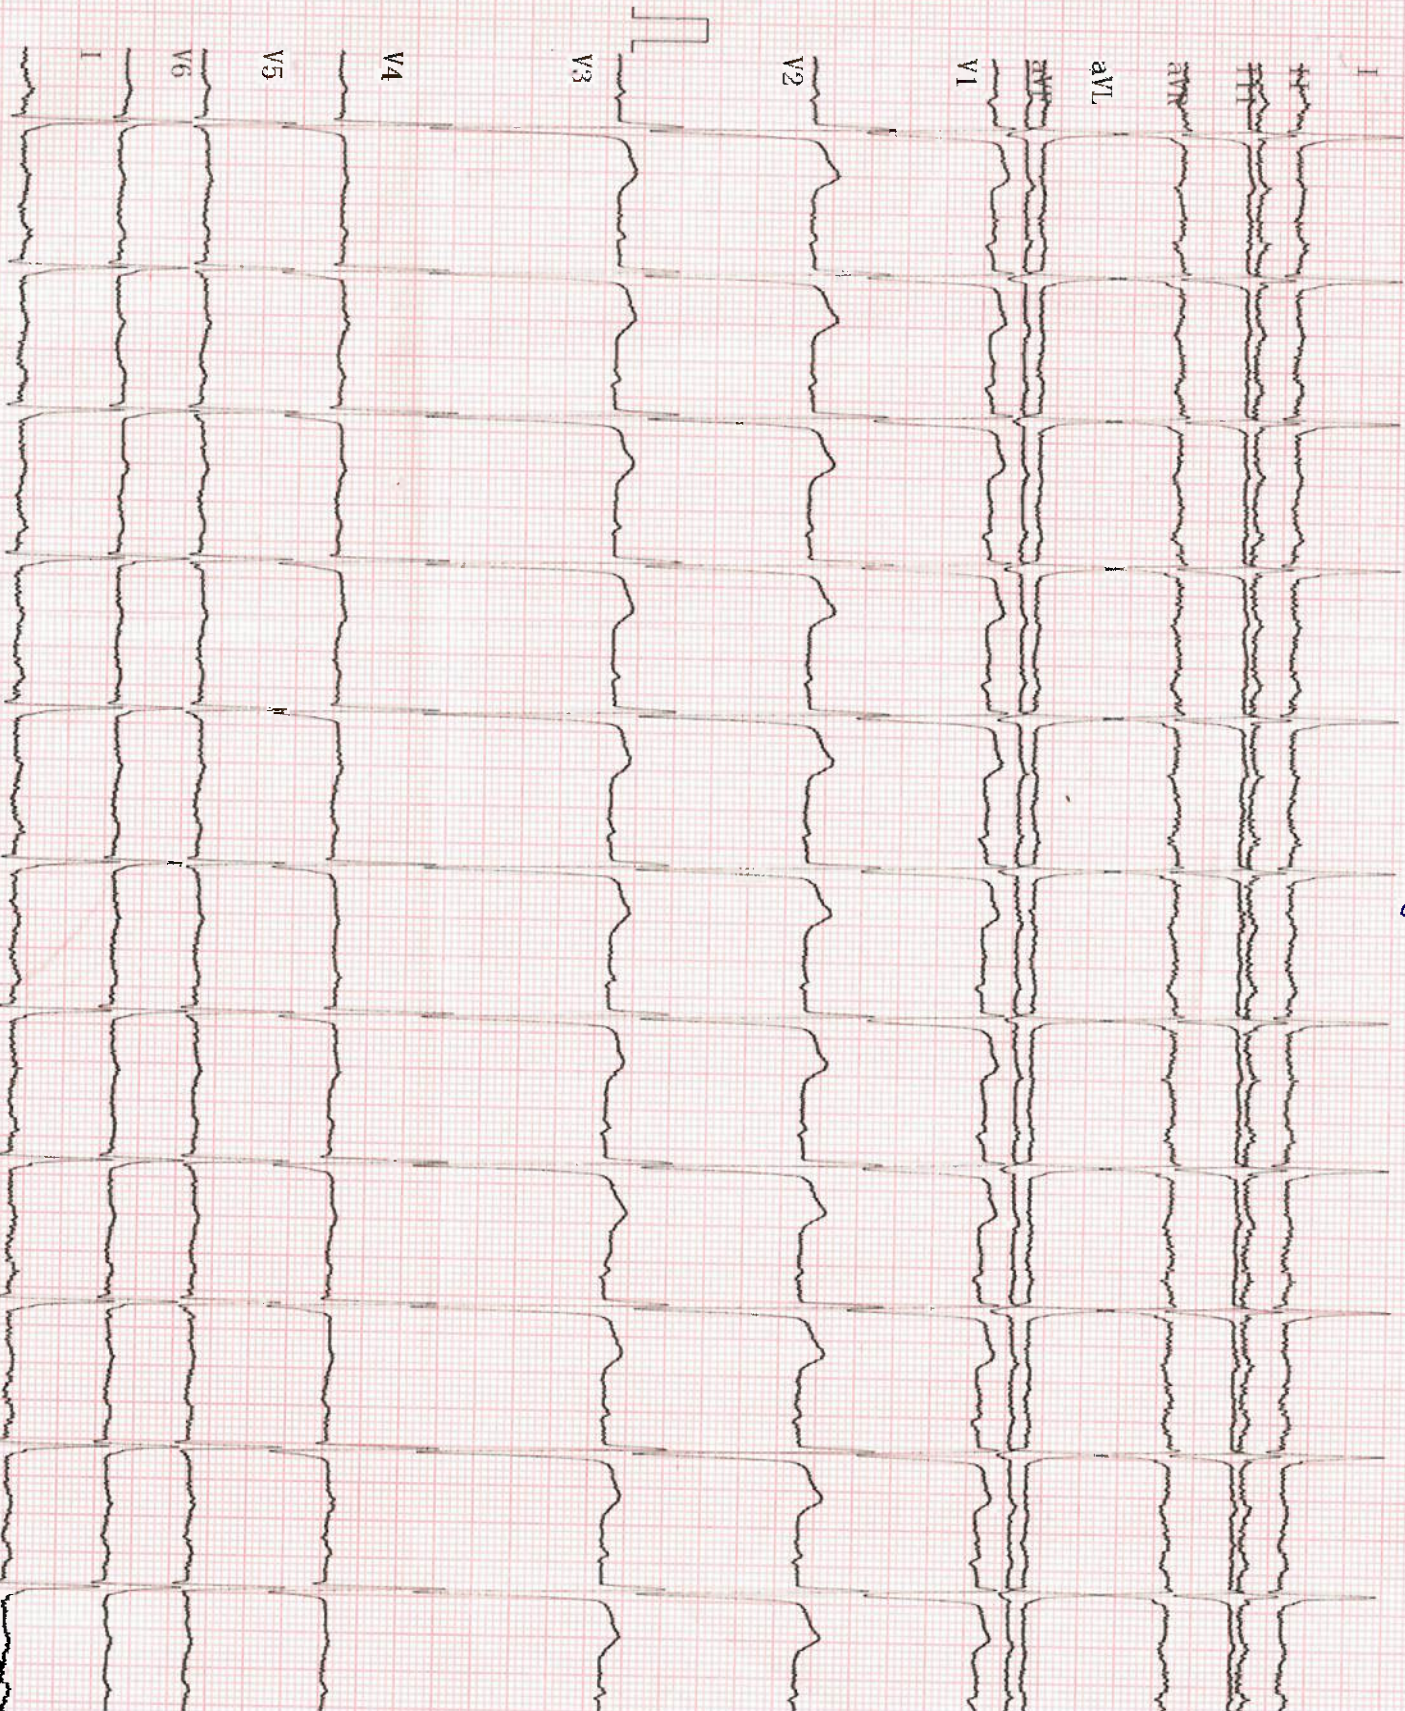

Velocidade: 25mm/s Filtro: H50 d 35Hz AC: 50 Hz BIOCARE ECG-1200 V4.06.000