


2025-08-08, 09:03

Real Tempo Modo

José Paulo Turtulano da Silva DN: 17/03/1973

10mm/mV

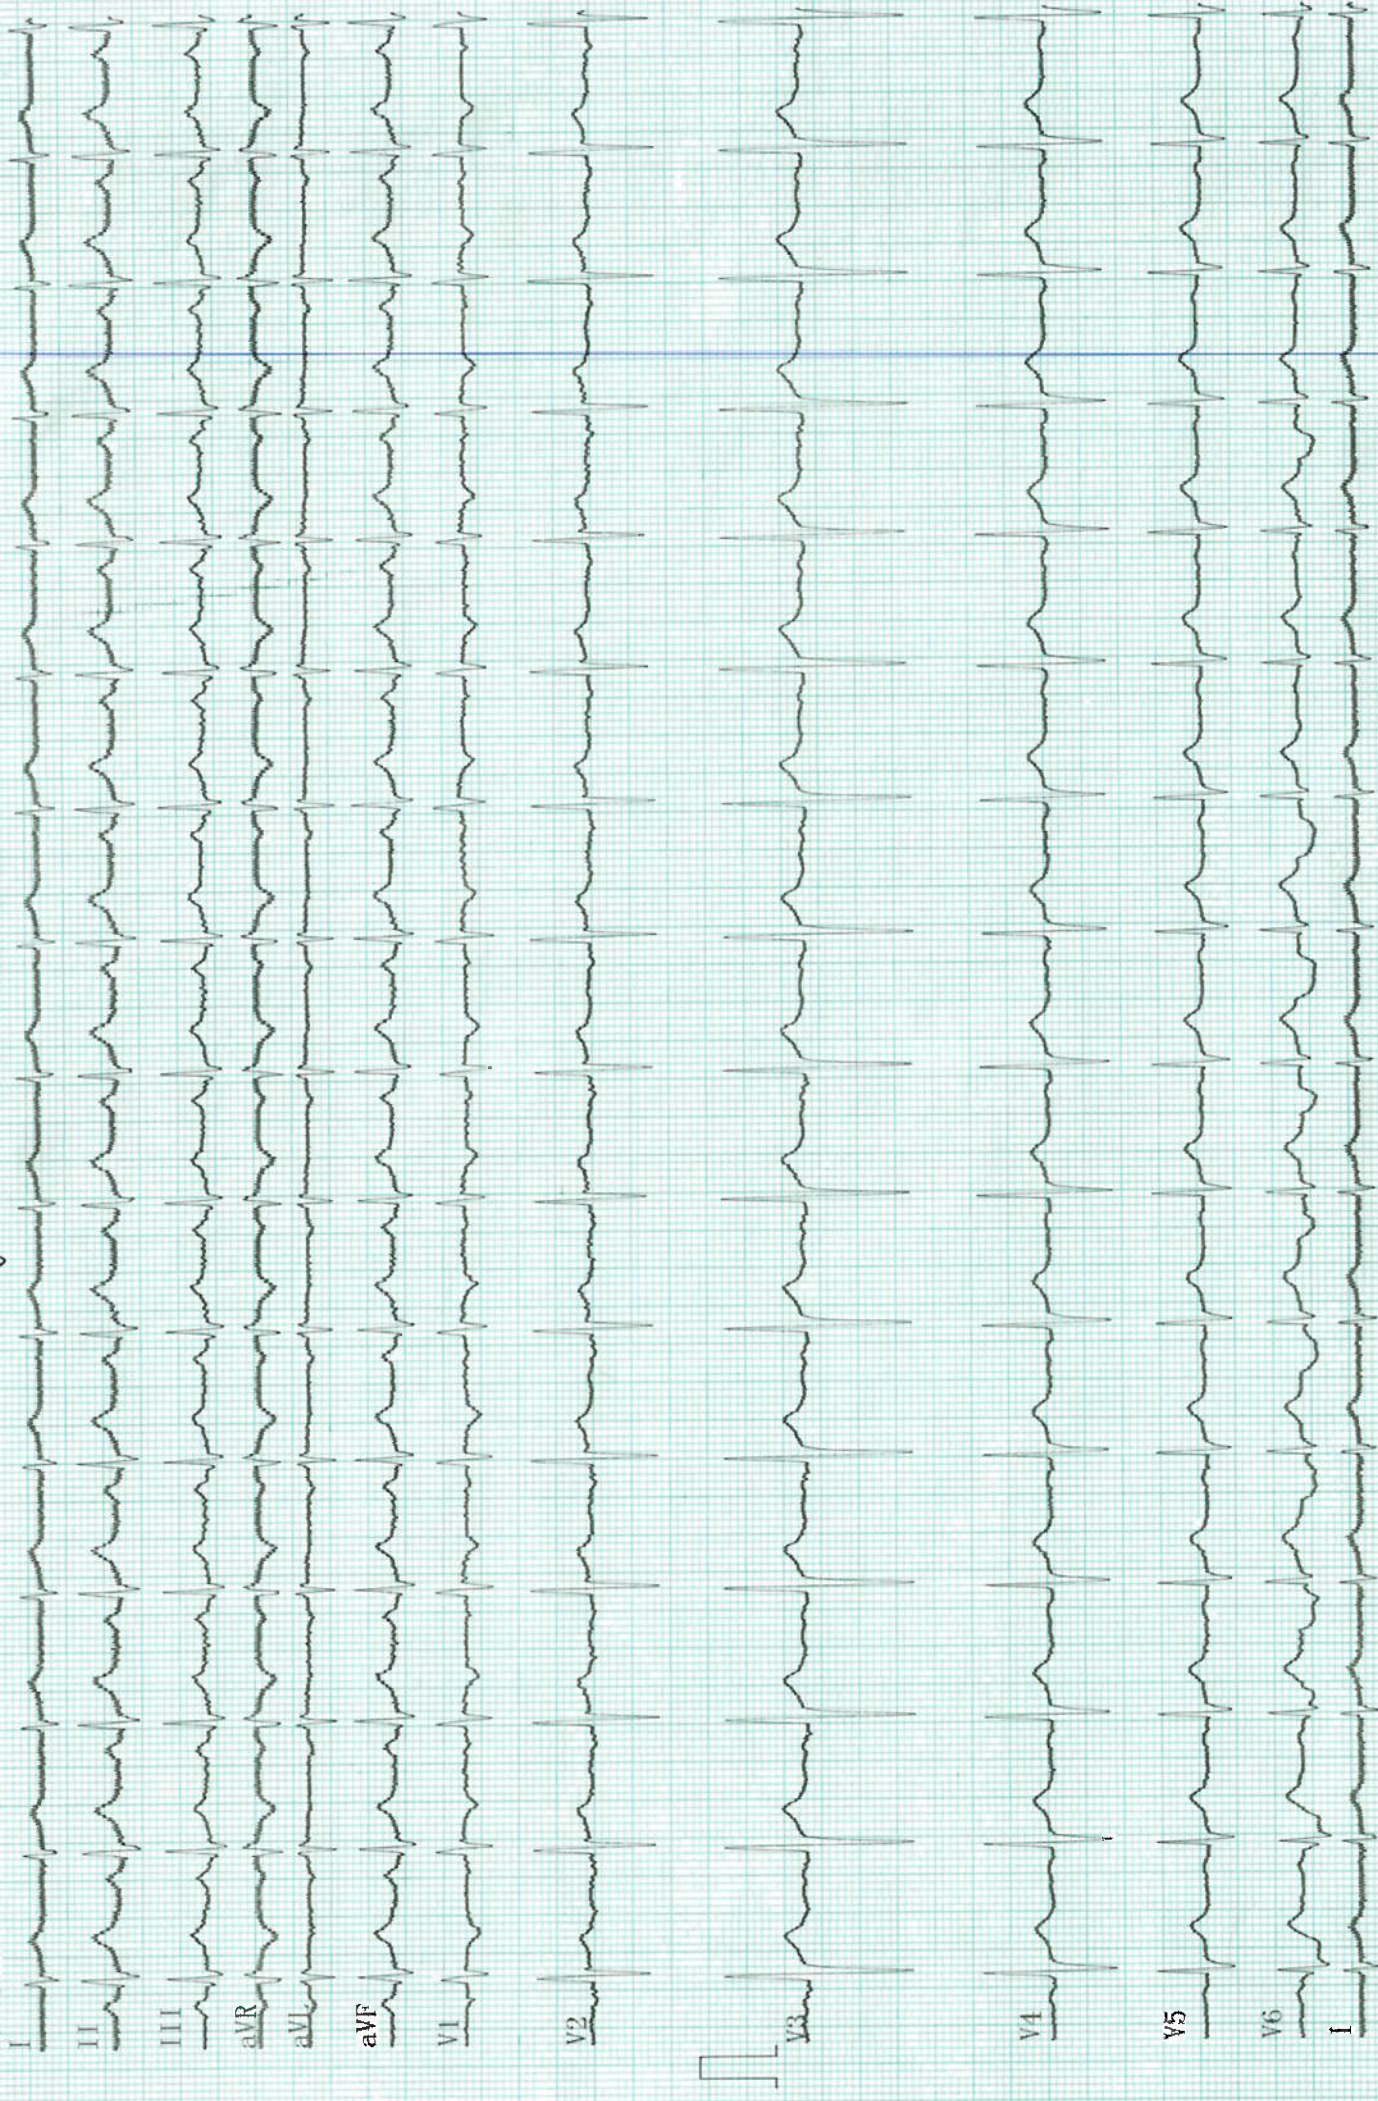

Velocidade: 25mm/s Filtro: H50 d 35Hz AC: 50 Hz BIO CARE ECG 1200 V4.06.000