


DN-191031-1972

Leonardo Ferreira da Lima

Real Tempo Modo

2025 08 01, 09:44

10mm/mV

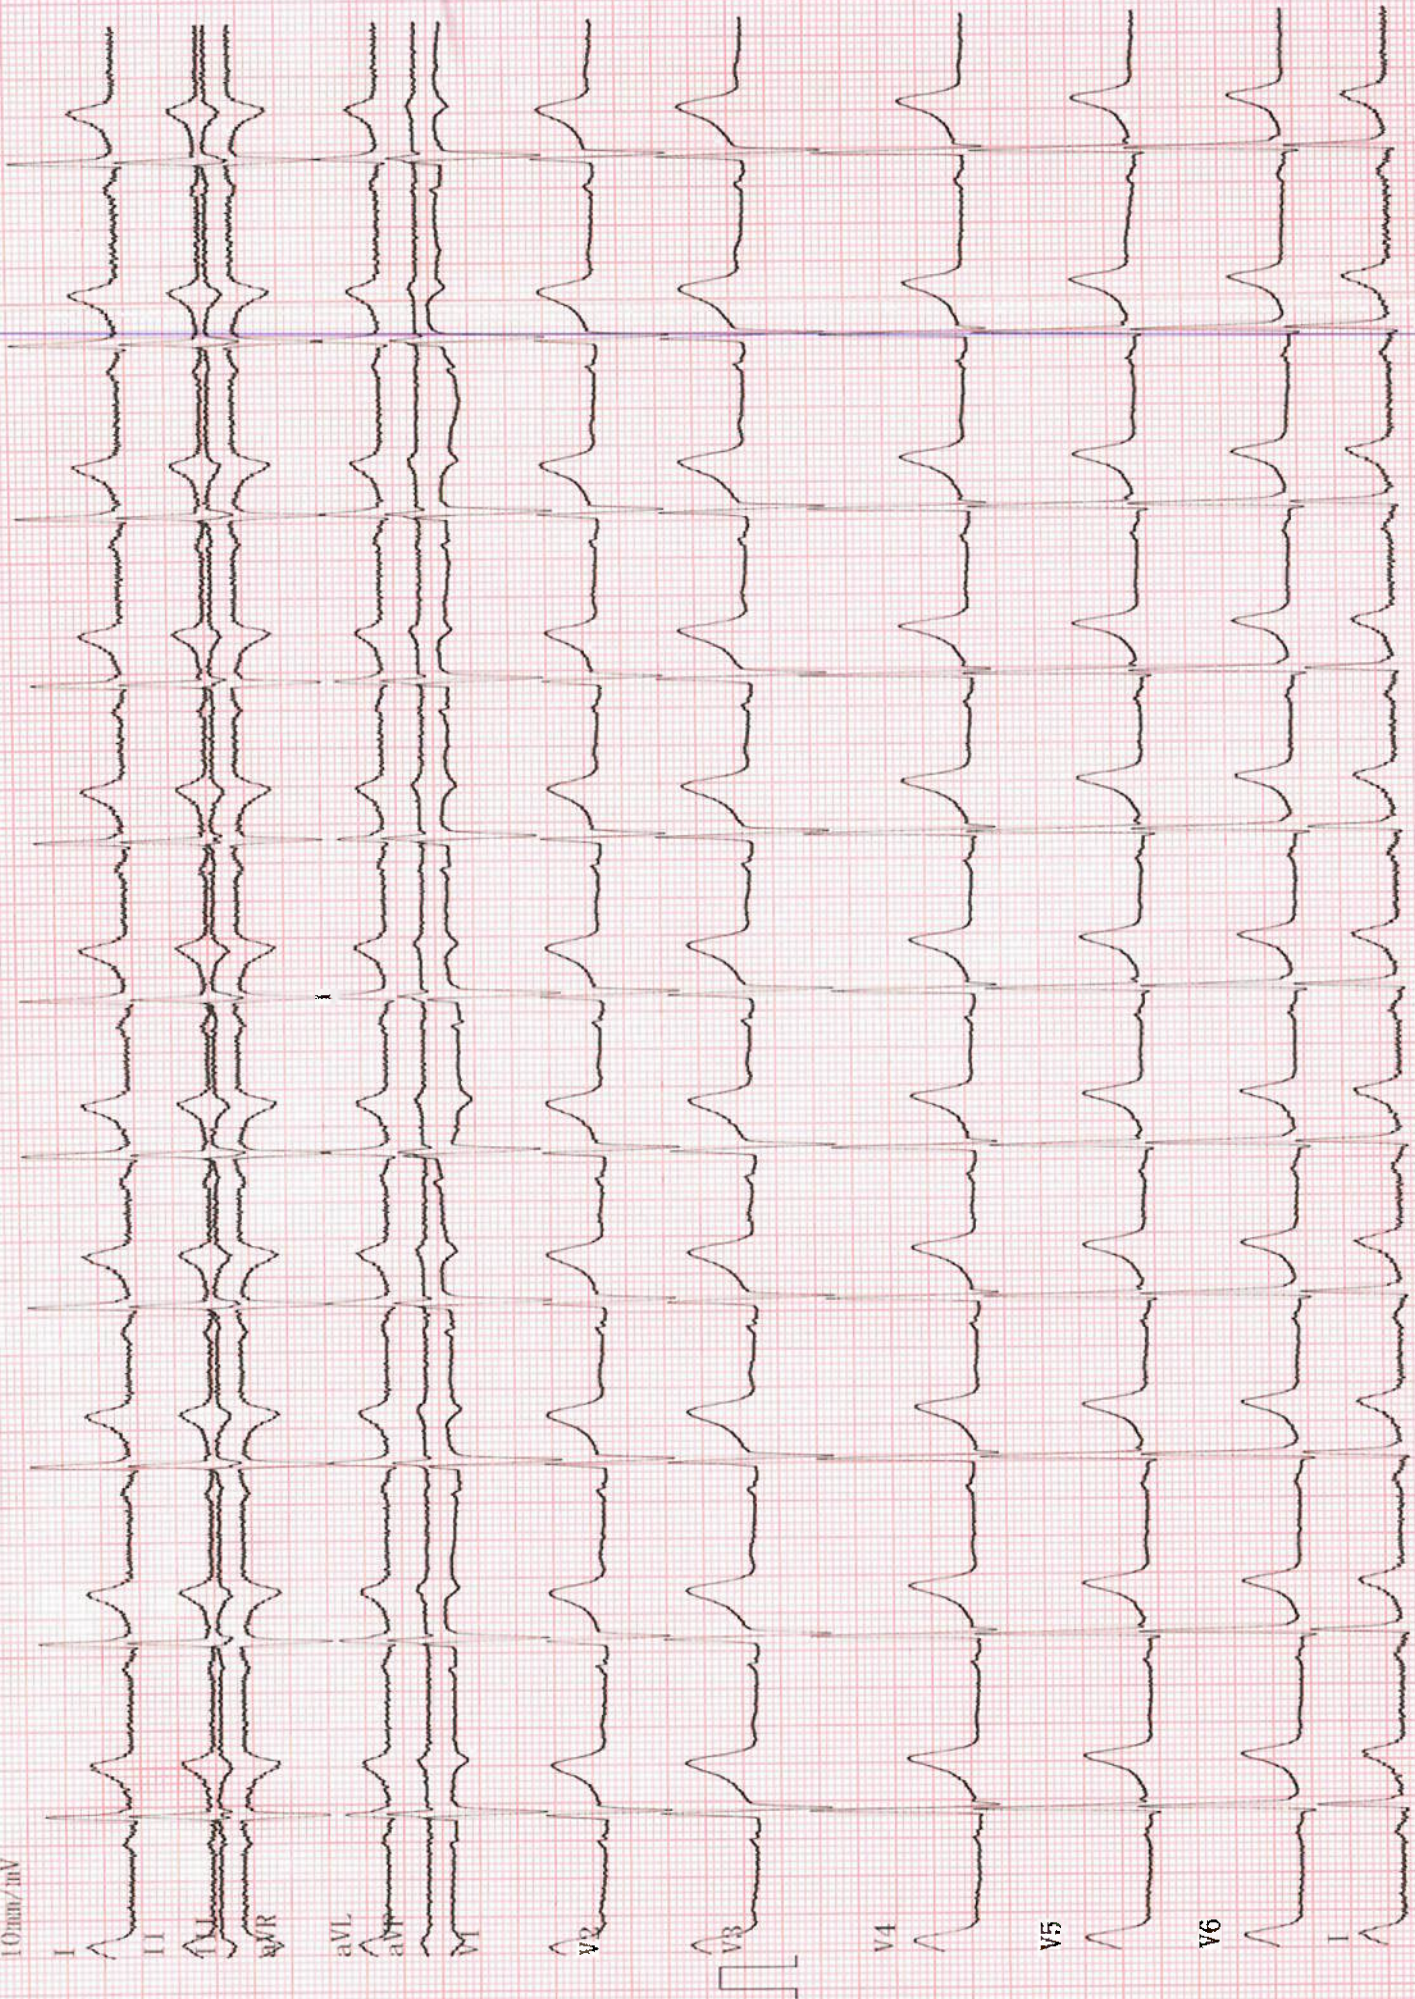

Velocidade: 25mm/s Filtro: 150 d 35Hz AC: 50 Hz BIOCARD ECG 1200 V4.06.000