


10. No.:

Luciano Alexandre de Siqueira

Impressão de 12 Canais
Freq. Cardíaca: 58 bpm

Hospital: SESI
Confirmado por:

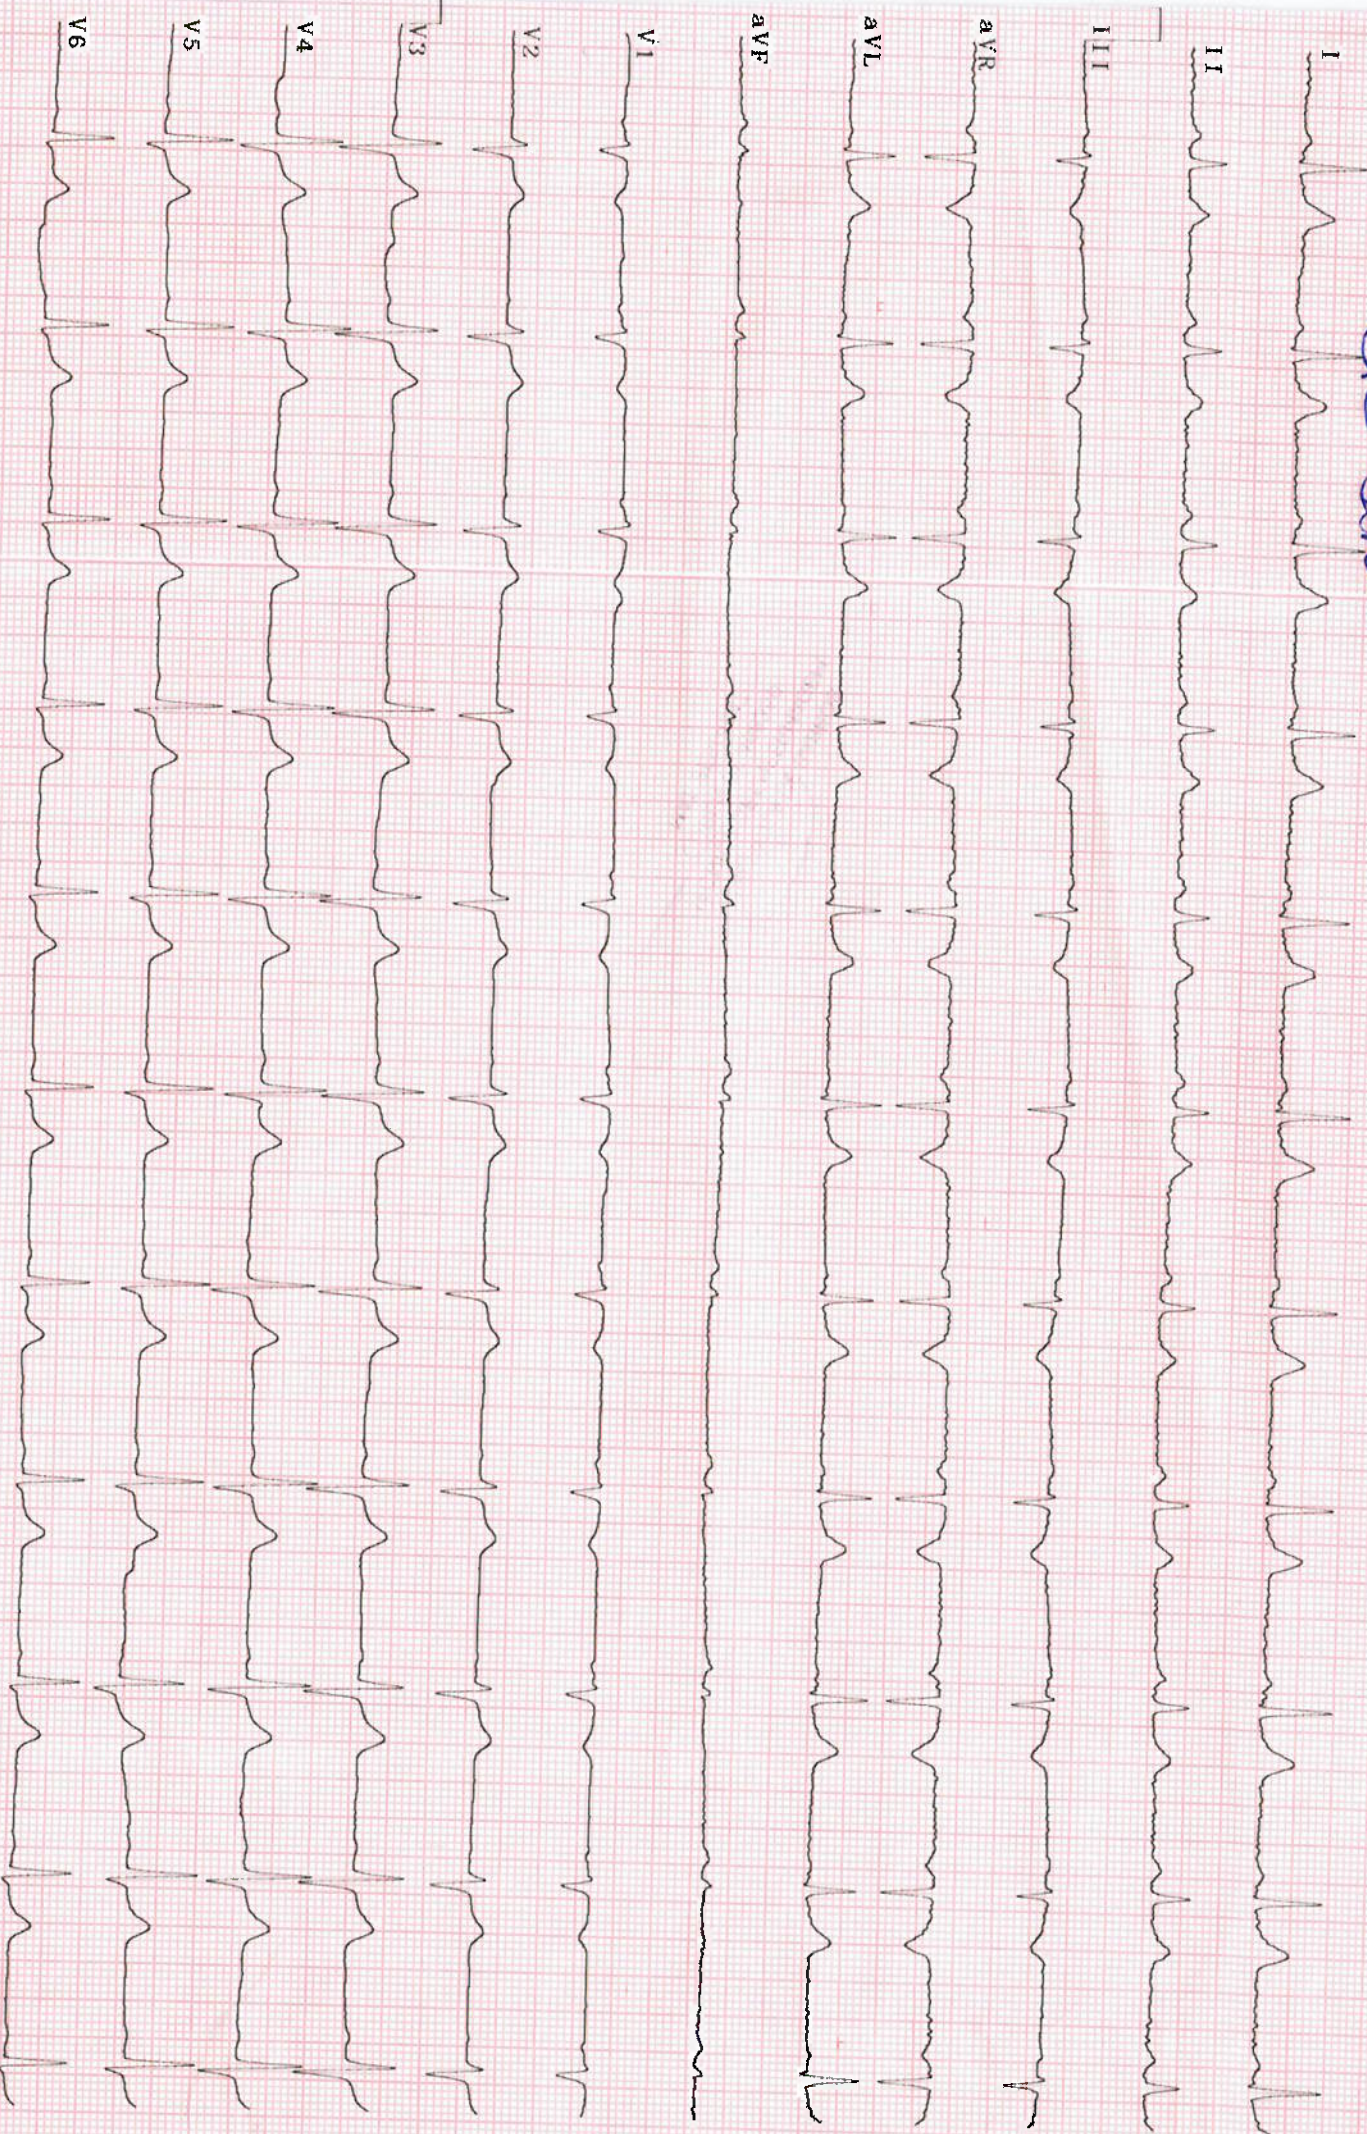

0.1Hz - 40Hz.

I-aVF: 10.0mm/mV, V1-V6: 5.0mm/mV. 25.0mm/sec.

CardioTouch6.11.30 Bionet Co., Ltd.