


2025-07-30, 09:08
0mm/mV

Real-Tempo Modo

Genildo Francisco de Souza 45a-02

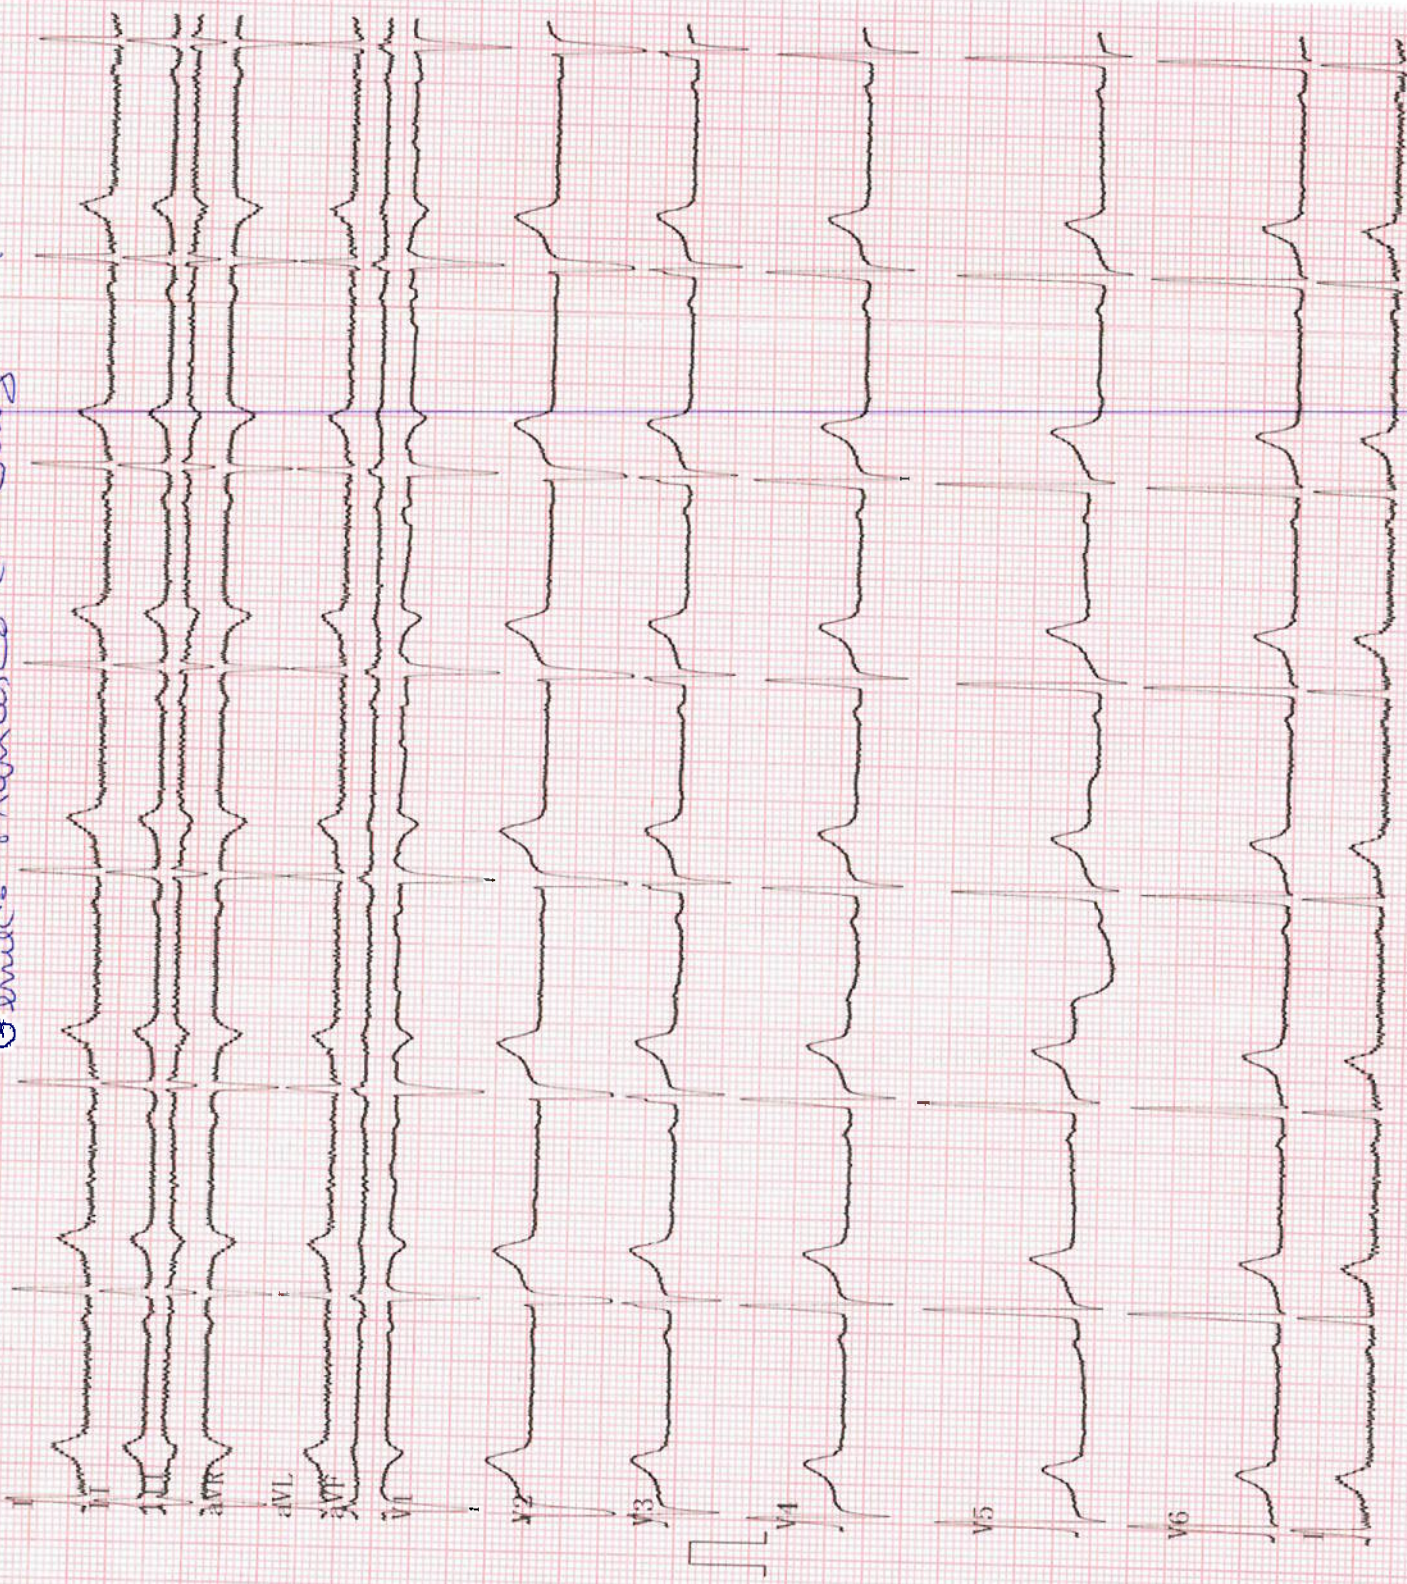

Velocidade: 25mm/s Filtro: H50 d 35Hz AC: 50 Hz BIOCare ECG 1200 V4.06.000