


2029-08-01, 08:53
10mm/mV

Real-Tempo Modo

Edmundo Almeida de Souza

DN. 25/03/1983

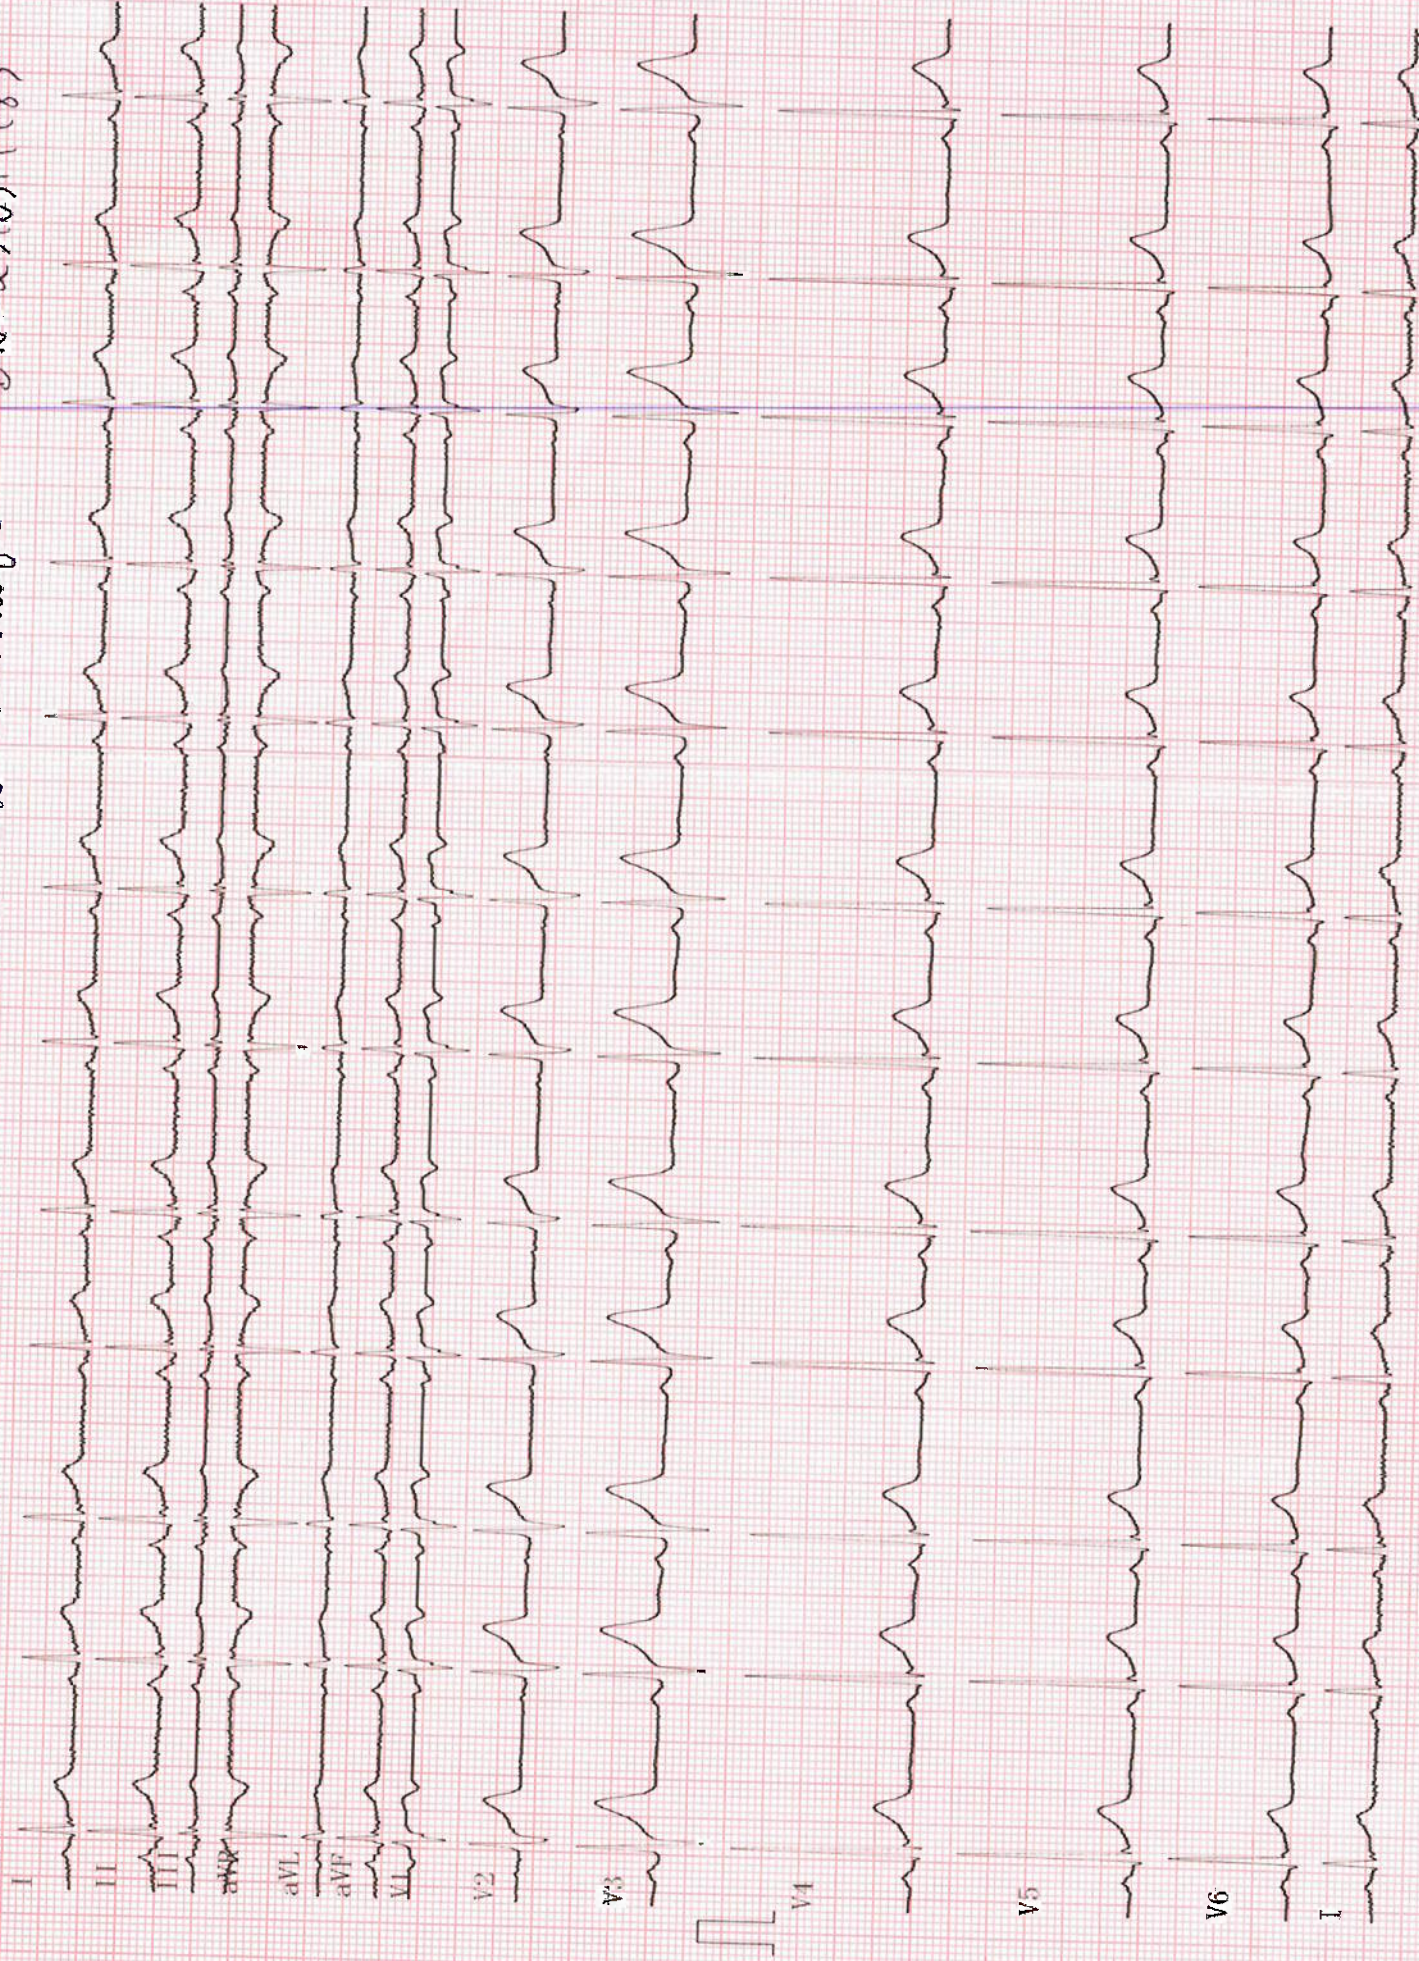

Velocidade: 25mm/s Filtro: 150 d 35Hz AC: 50 Hz BIOTACRE ECG 1200 V4.06.000