


2025-08-04, 12:28
10mm/mV

Real-Tempo Monitor

Gronson Julio noelcarant 330m

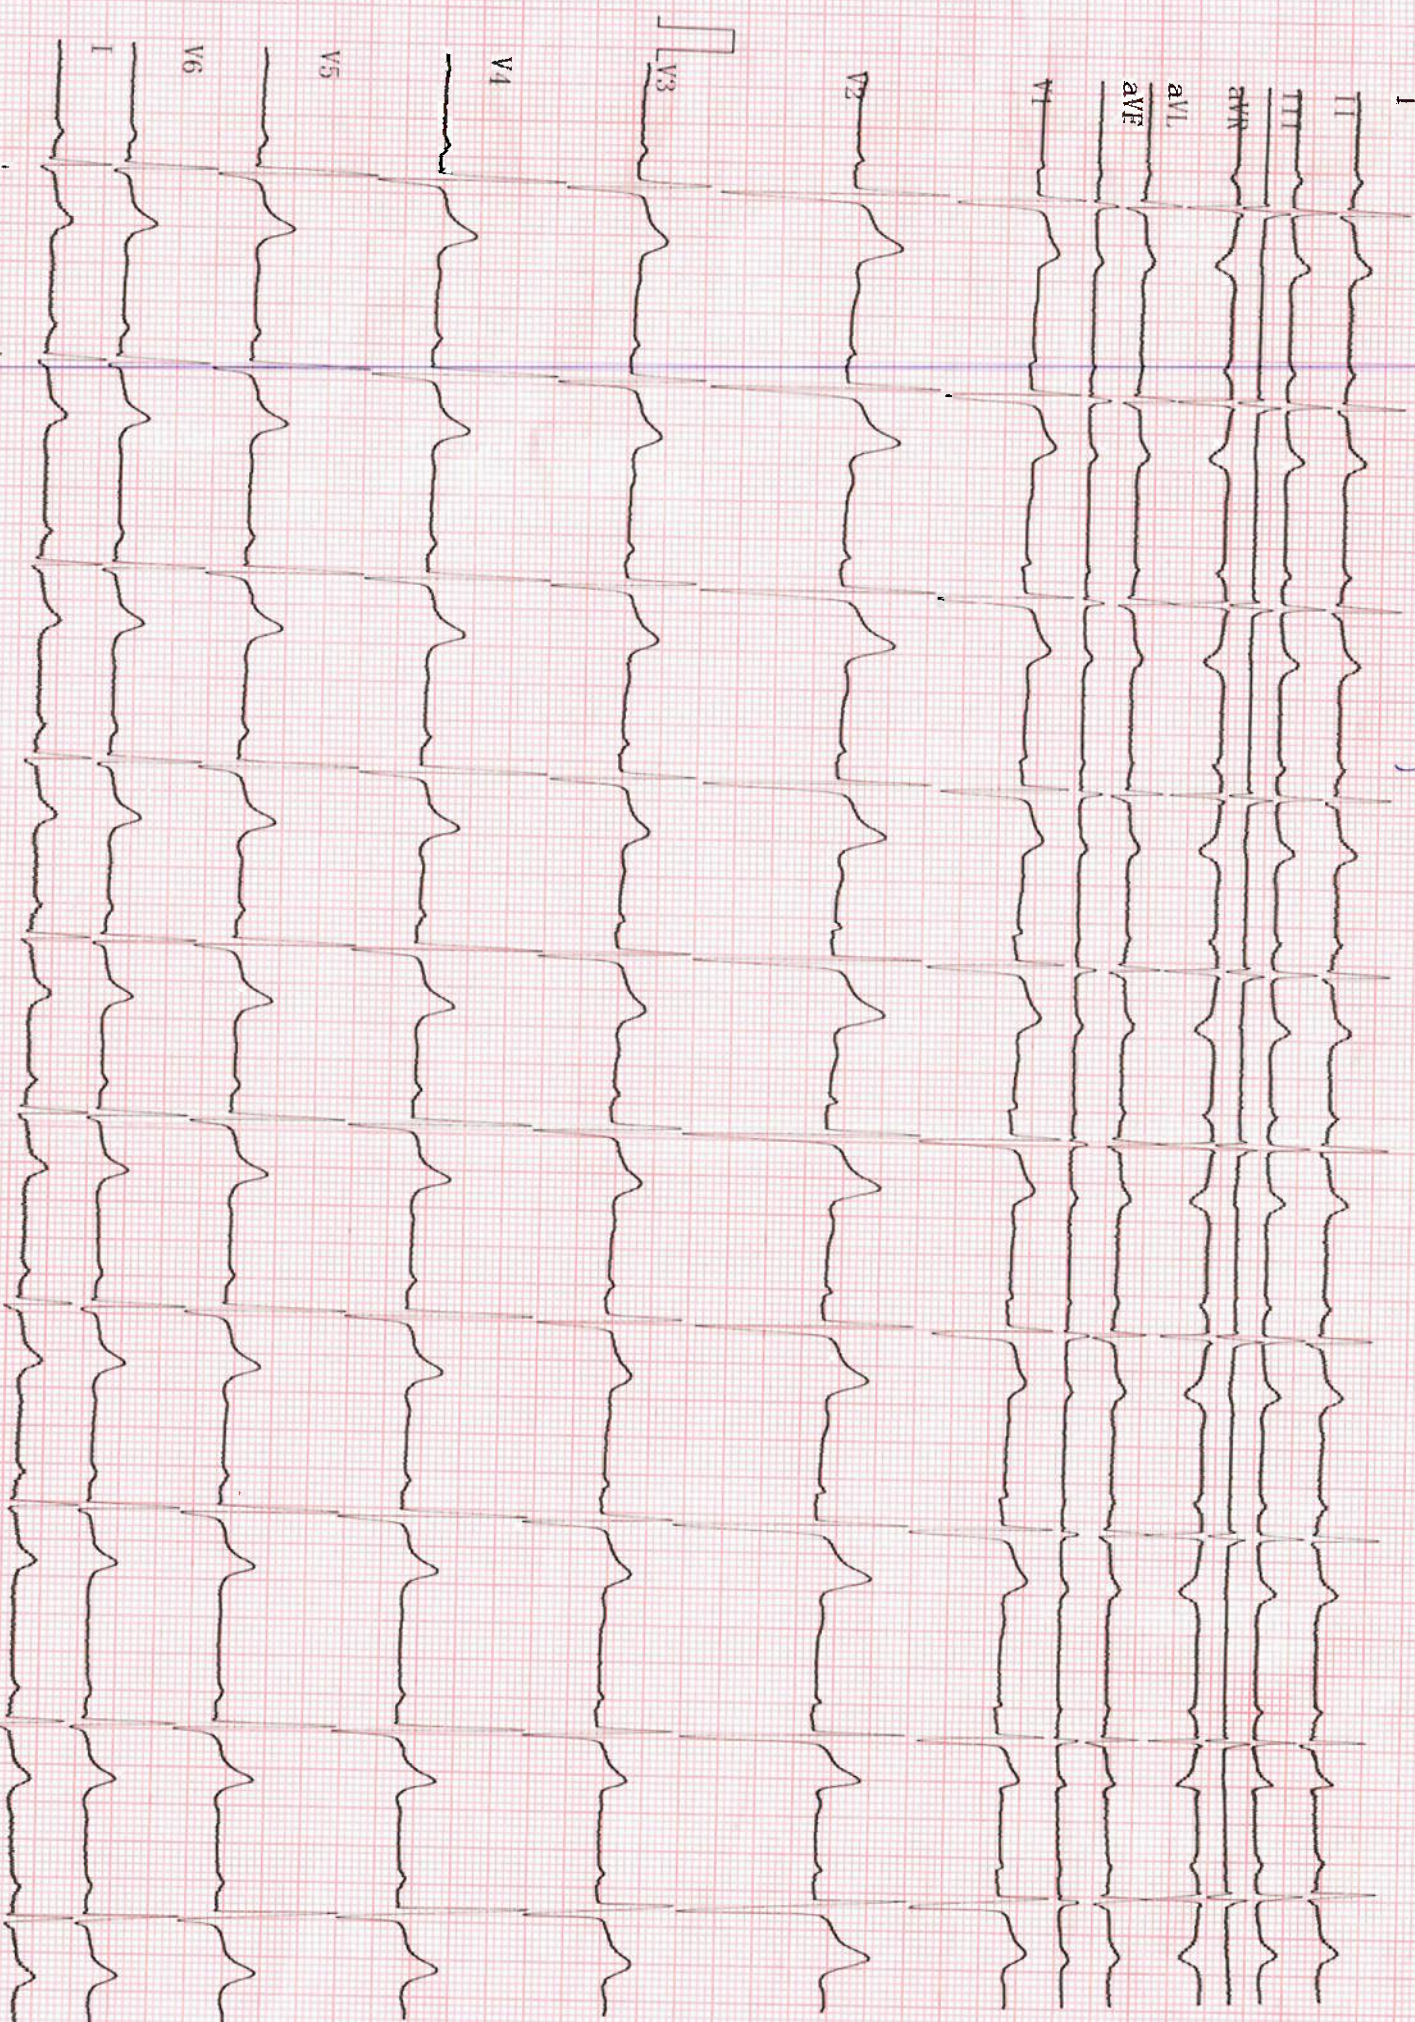

Velocidade: 25mm/s Filtro: H50 d 35Hz AC: 50 Hz BIOCARD ECG 1200 V1.06.000