


2025-08-11, 09:39

Real-Time Modo

Flavio Sales da Rocha Souza 25 ans

1.0mm/mV

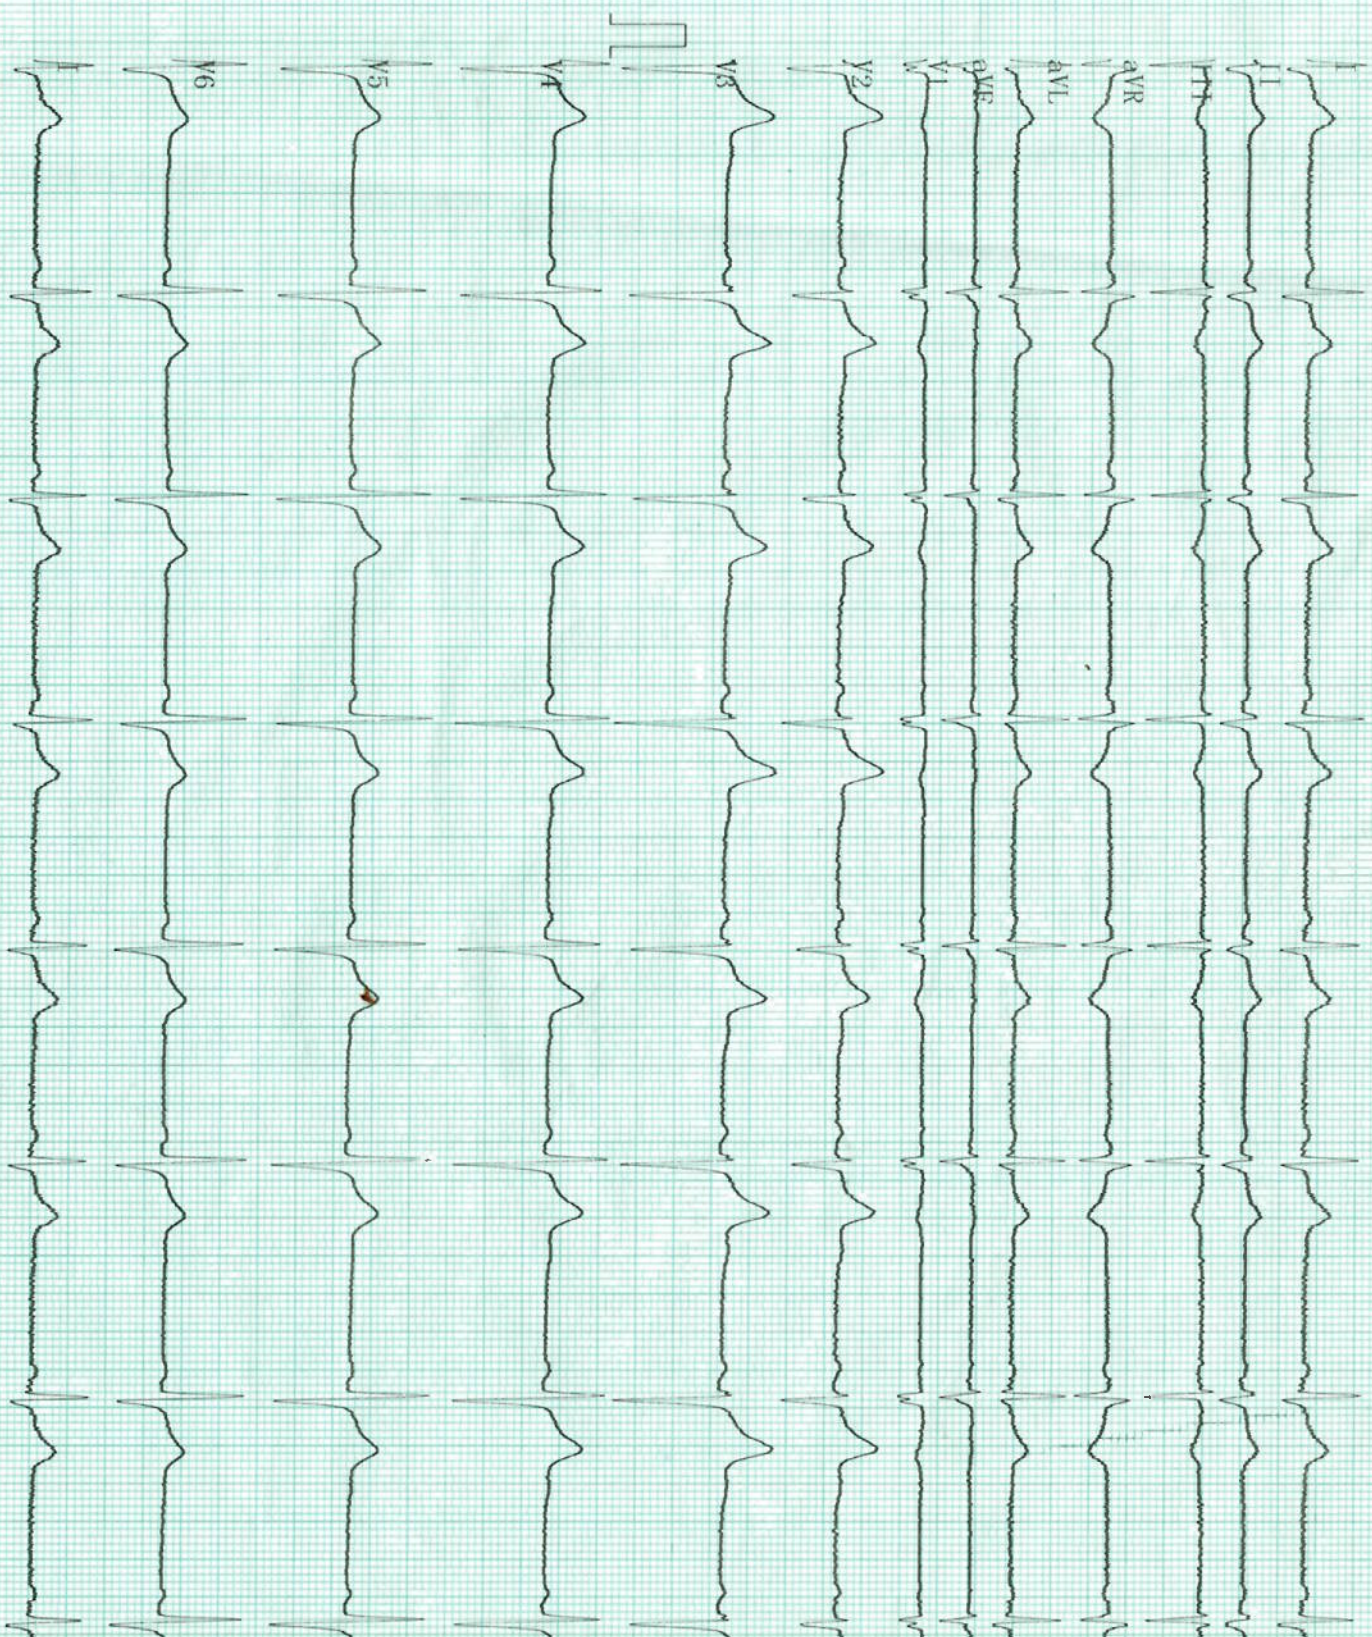

Velocidade: 25mm/s Filtro: H50 d 35Hz AC: 50 Hz BIOCARE ECG-1200 V4.06.000