

2025-08-06 07:40:44

ID:


Nome:

Silvio Gouveia de C'

Impressão de 12 canais

Freq. Cardíaca: 57 bpm

Hospital: SESI
Confirmado por:

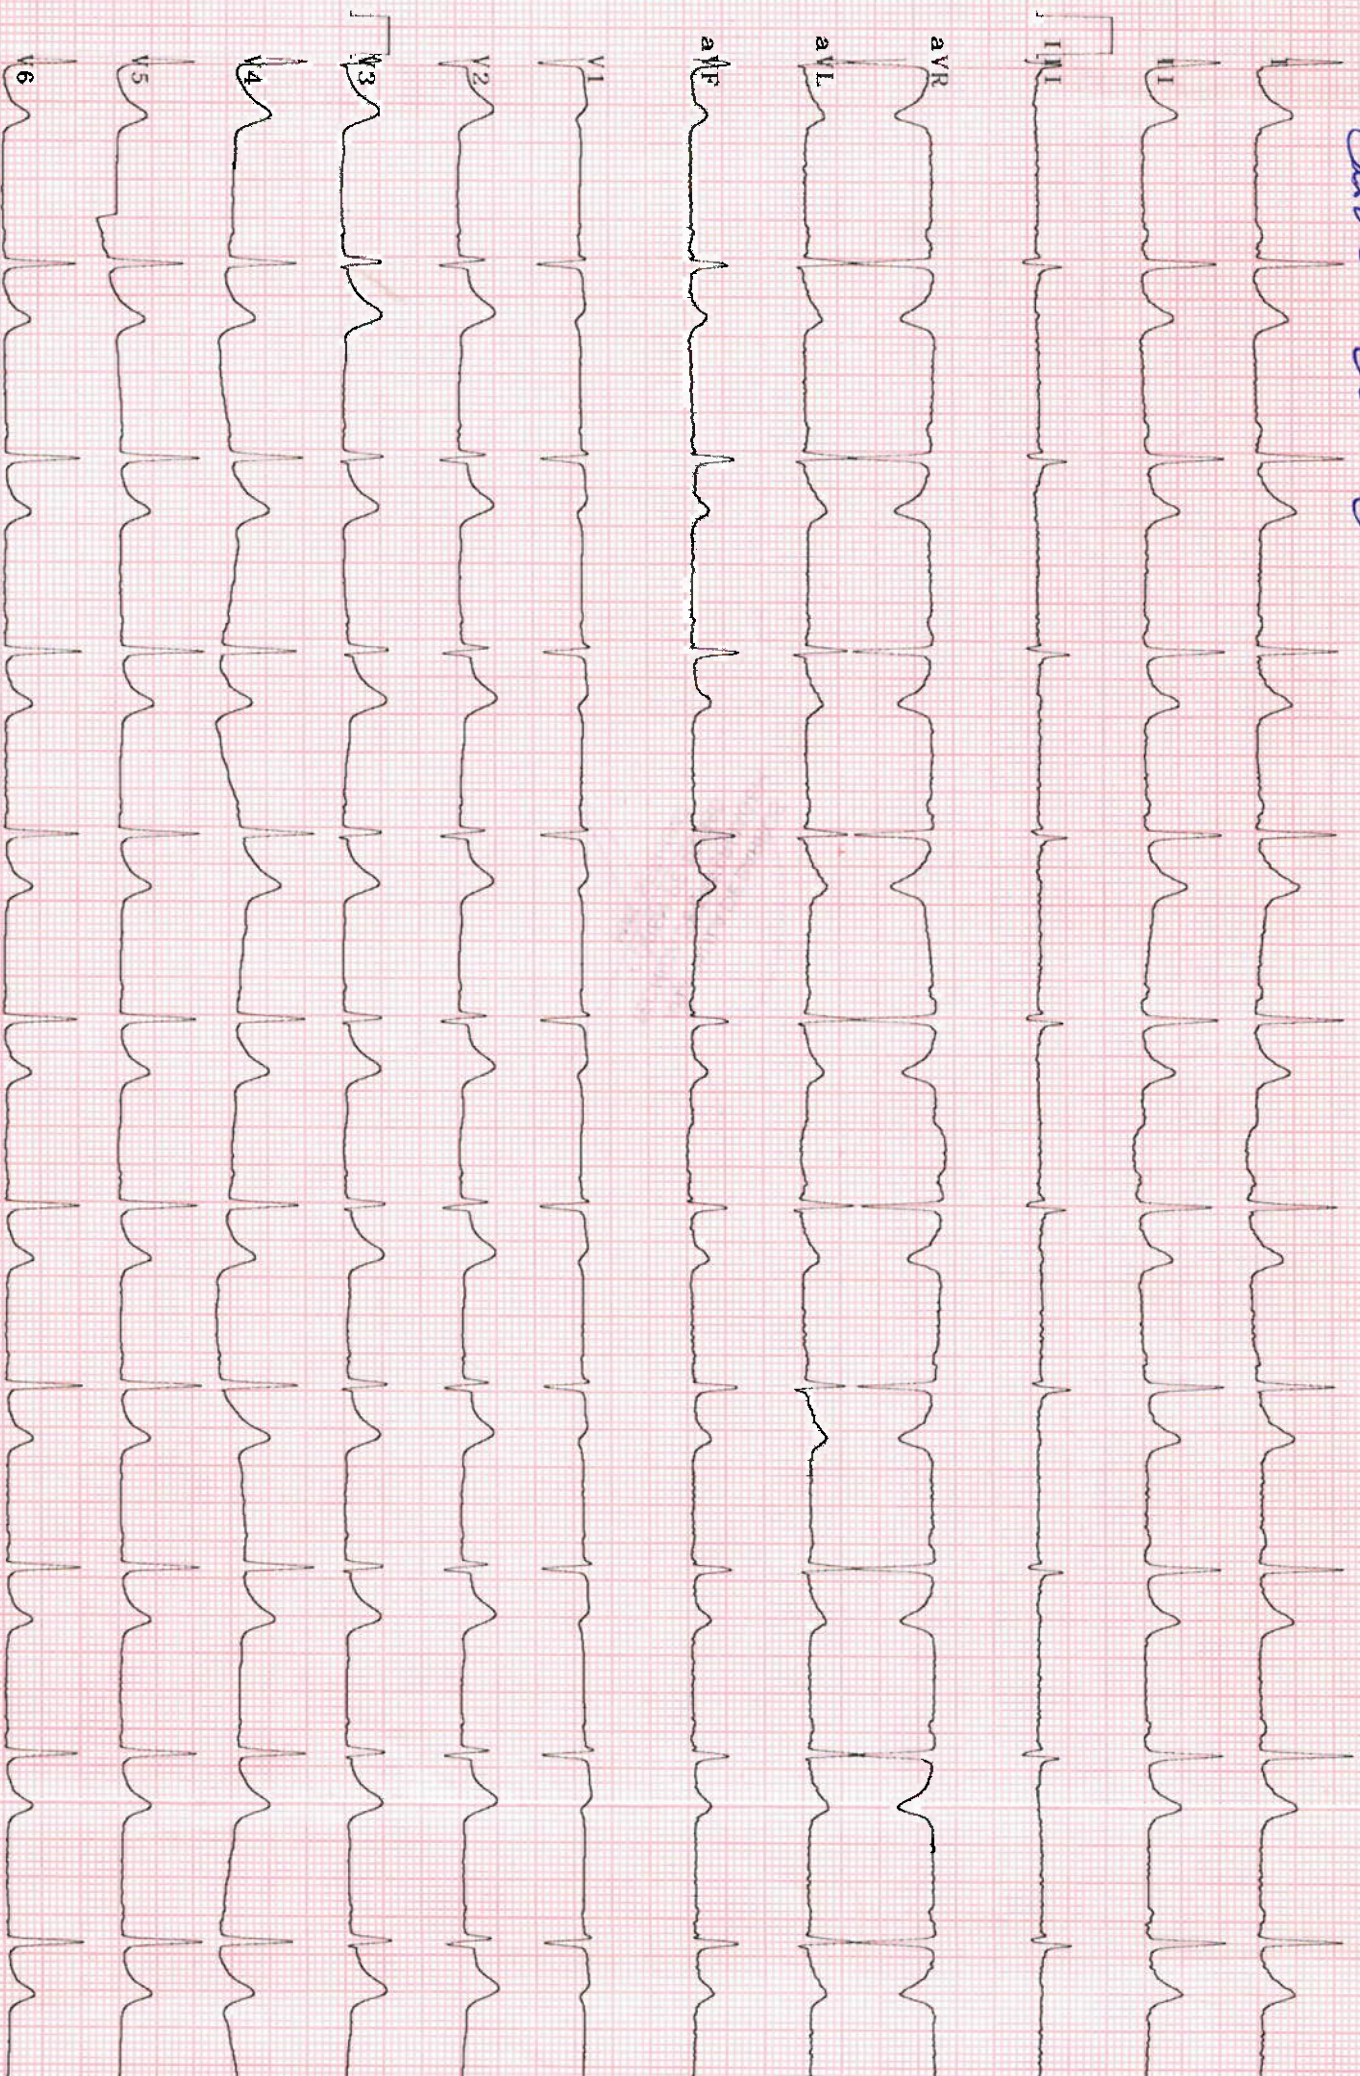

0.1Hz - 40Hz.

I-aVF: 10.0mm/mV, V1-V6: 5.0mm/mV, 25.0mm/seg.

CardioTouch6.11.30 Bionet Co., Ltd.