


2025-07-21, 10:00

Real Tempo Modo *duis* Fernando de Silva e Silva 22000

10mm/mV

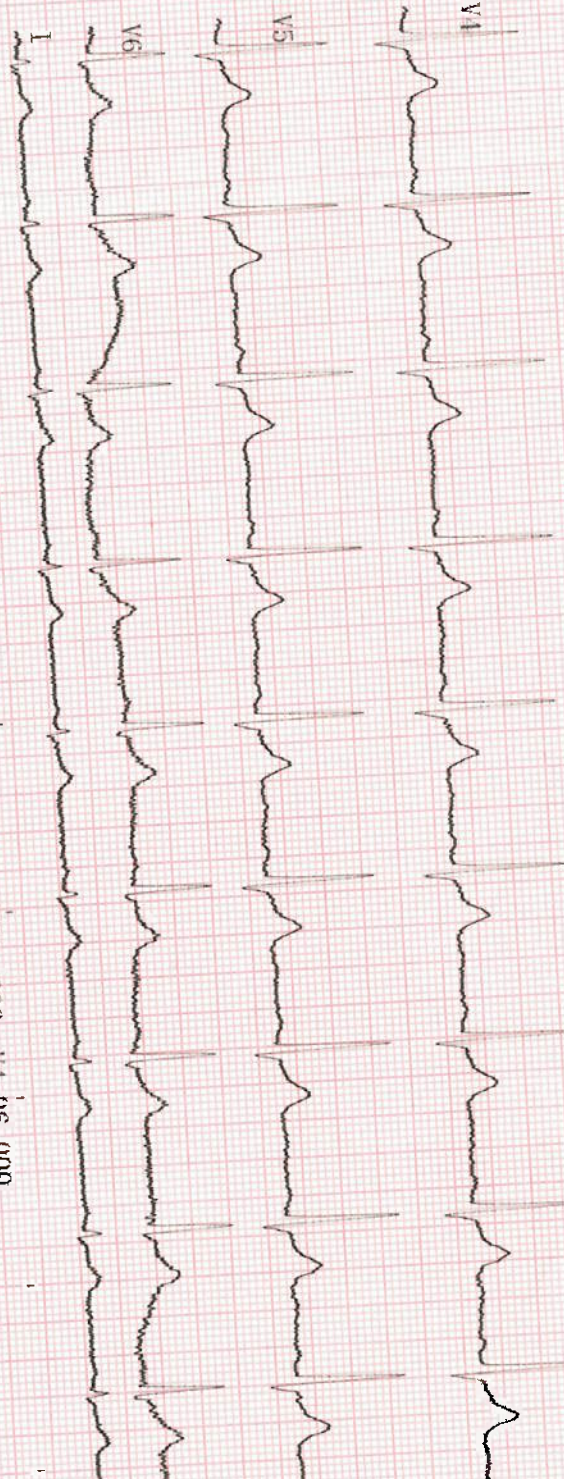

Velocidade: 25mm/s Filtro: H50 d 35Hz AC: 50 Hz BIOCARE ECG-1200 V4.06.000